



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Hasselbring's Harmony Ranch/Patty Hasselbring  
29049 Davis Road  
Concordia MO 64020 USA

**Date:** 06/10/19  
**Shear ID:** 186145  
**Test No:** 975737


### Animal and Sample Description

**Animal Name:** Mont Everest  
**ARI #:** 35373445  
**Breed:** Alpaca(Suri)  
**Sex:** Male  
**Color:** White

**Date of Birth (Age):** 06/28/2018  
**Sample Location:** Side  
**Sample Date:** 05/15/2019  
**Previous Shear Date:** XX/XX/XX  
**Total Fleece Wt (lbs):** 4.50

### Laboratory Data

<b>Mean Fiber Diameter:</b>	19.9 microns	<b>Mean Staple Length:</b>	192.8 mm
<b>Standard Deviation:</b>	3.8 microns	<b>Length Standard Deviation:</b>	6.3 mm
<b>Coefficient of Variation:</b>	19.1 %	<b>Length Coefficient of Variation:</b>	3.3 %
<b>Spin Fineness:</b>	19.1 microns	<b>Mean Curvature:</b>	14.2 deg/mm
<b>Fibers Greater Than 30 microns:</b>	1.1 %	<b>SD Curvature:</b>	17.2 deg/mm
<b>Comfort Factor:</b>	98.9 %	<b>Medullated Fibers:</b>	1.0 %

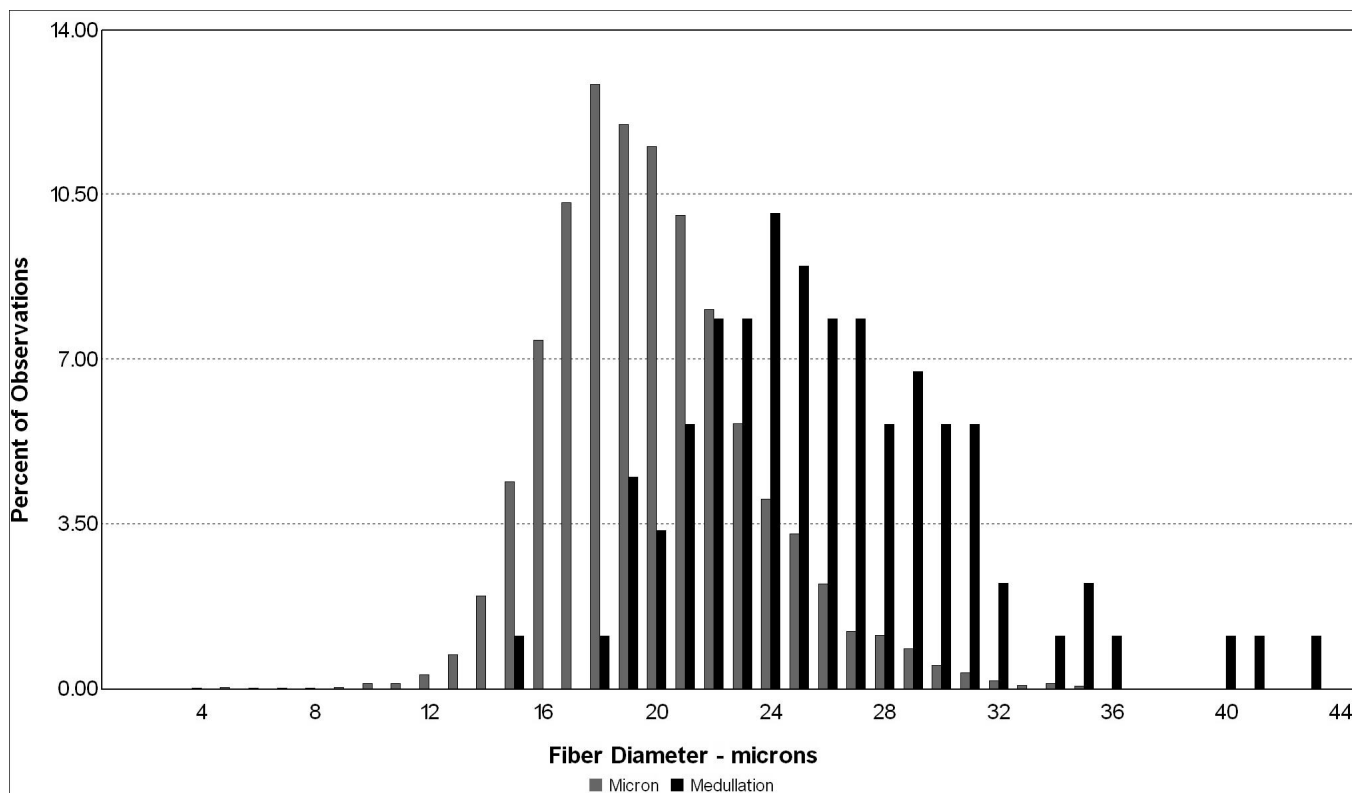

This Test Performed According to I.W.T.O Method 47