

## Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

### Sirolan Laserscan Micron Test Report

Rockford Bay Ranch/Kathryn Pinkerton  
14701 S Heritage Dr  
Coeur d'Alene ID 83814

09/14/10

Test No: 391090


#### Animal and Sample Description

**Animal Name:** NHM KayCee  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** MB

**Animal ID:** 824742  
**Sample Location:** Side  
**Sample Date:** 05/08/10  
**Age:** 07/06/00

#### Laboratory Data

**Mean Fiber Diameter:** 23.3 microns  
**Standard Deviation:** 5.2 microns  
**Coefficient of Variation:** 22.3 %  
**Fibers Greater Than 30 microns:** 9.4 %

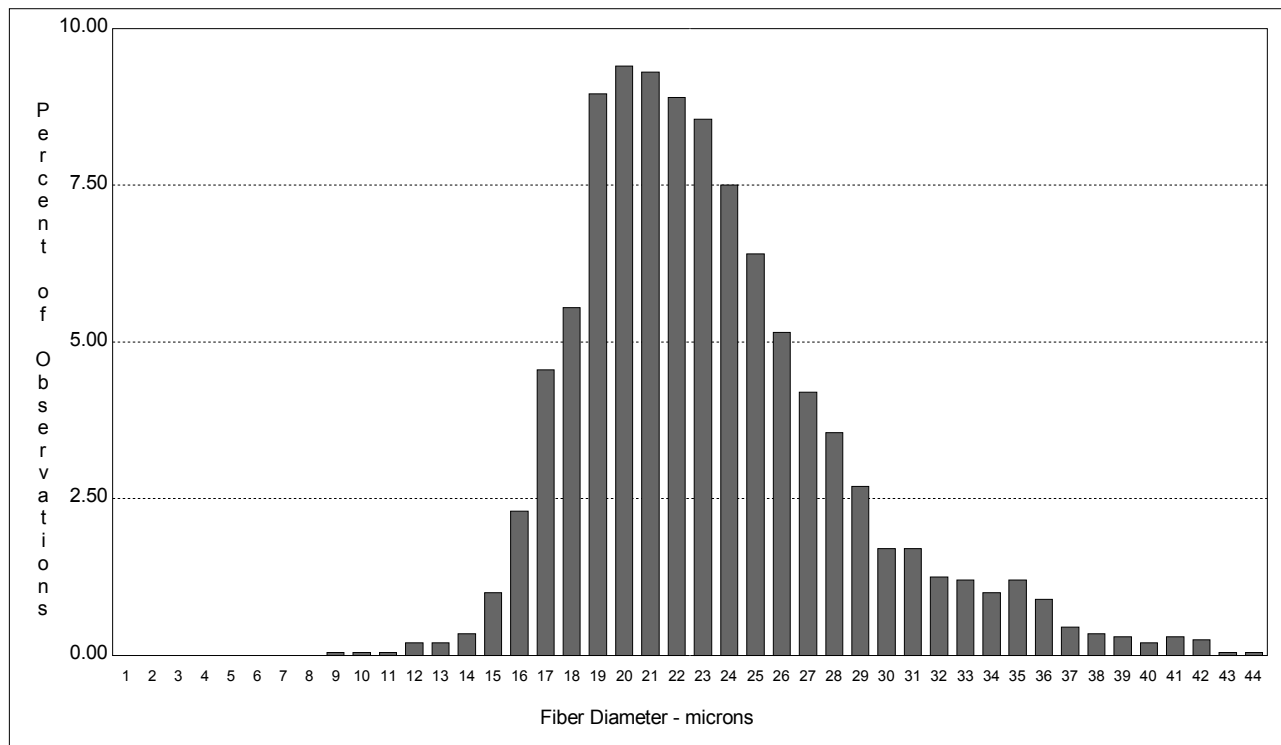

This Test Performed According to I.W.T.O Method 12