

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Rockford Bay Ranch/Kathryn Pinkerton
14701 S Heritage Dr
Coeur d'Alene ID 83814

09/14/10

Test No: 391089


Animal and Sample Description

Animal Name: Meteor
Breed: Alpaca(Huacaya)
Sex: Male
Color: DB/BB

Animal ID: 31864671
Sample Location: Side
Sample Date: 05/08/10
Age: 01/15/10

Laboratory Data

Mean Fiber Diameter: 18.7 microns
Standard Deviation: 4.3 microns
Coefficient of Variation: 22.9 %
Fibers Greater Than 30 microns: 1.5 %

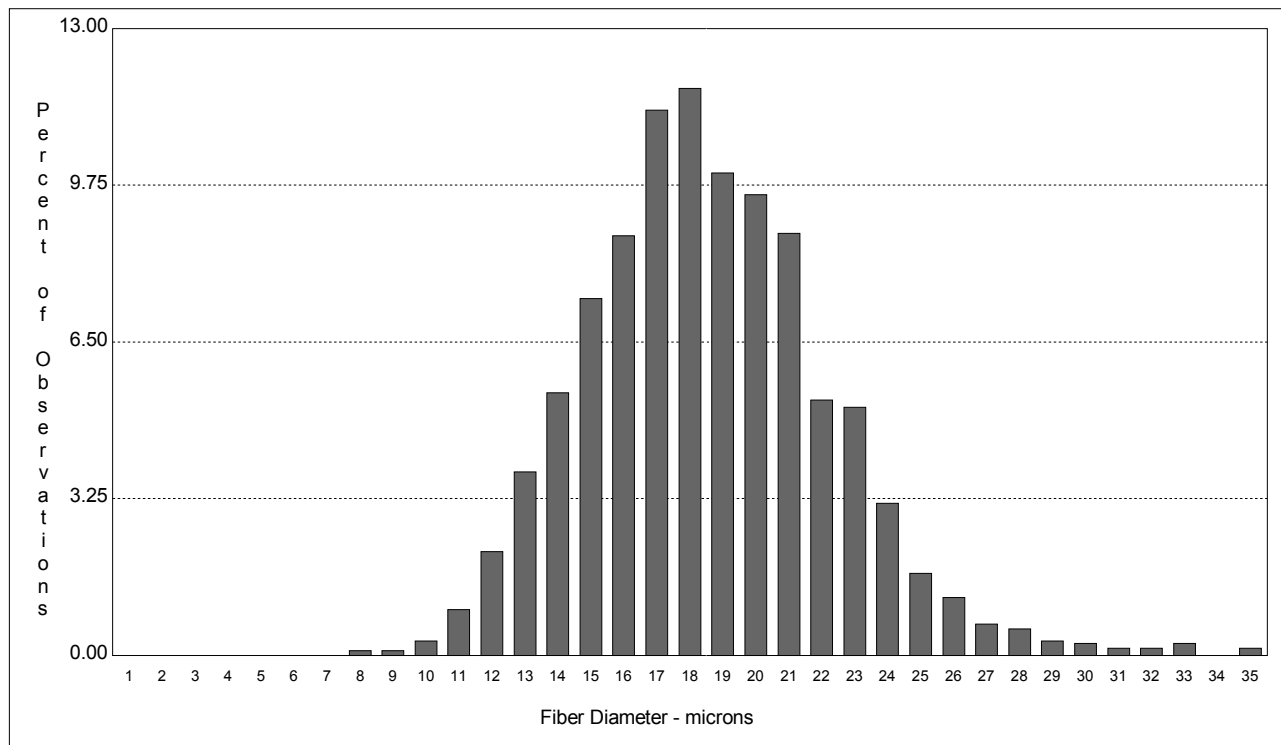

This Test Performed According to I.W.T.O Method 12