



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Rockford Bay Ranch/Esther Pinkerton  
14701 S Heritage Dr  
Coeur d'Alene ID 83814

03/04/20

Test No: 987577


### Animal and Sample Description

**Animal Name:** Rockford Rosaria Celeste  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Beige

**Animal ID:** XXXXX  
**Sample Location:** Side  
**Sample Date:** 05/24/19  
**Age:** 06/15/17

### Laboratory Data

**Mean Fiber Diameter:** 20.0 microns  
**Standard Deviation:** 4.5 microns  
**Coefficient of Variation:** 22.4 %  
**Fibers Greater Than 30 microns:** 3.1 %

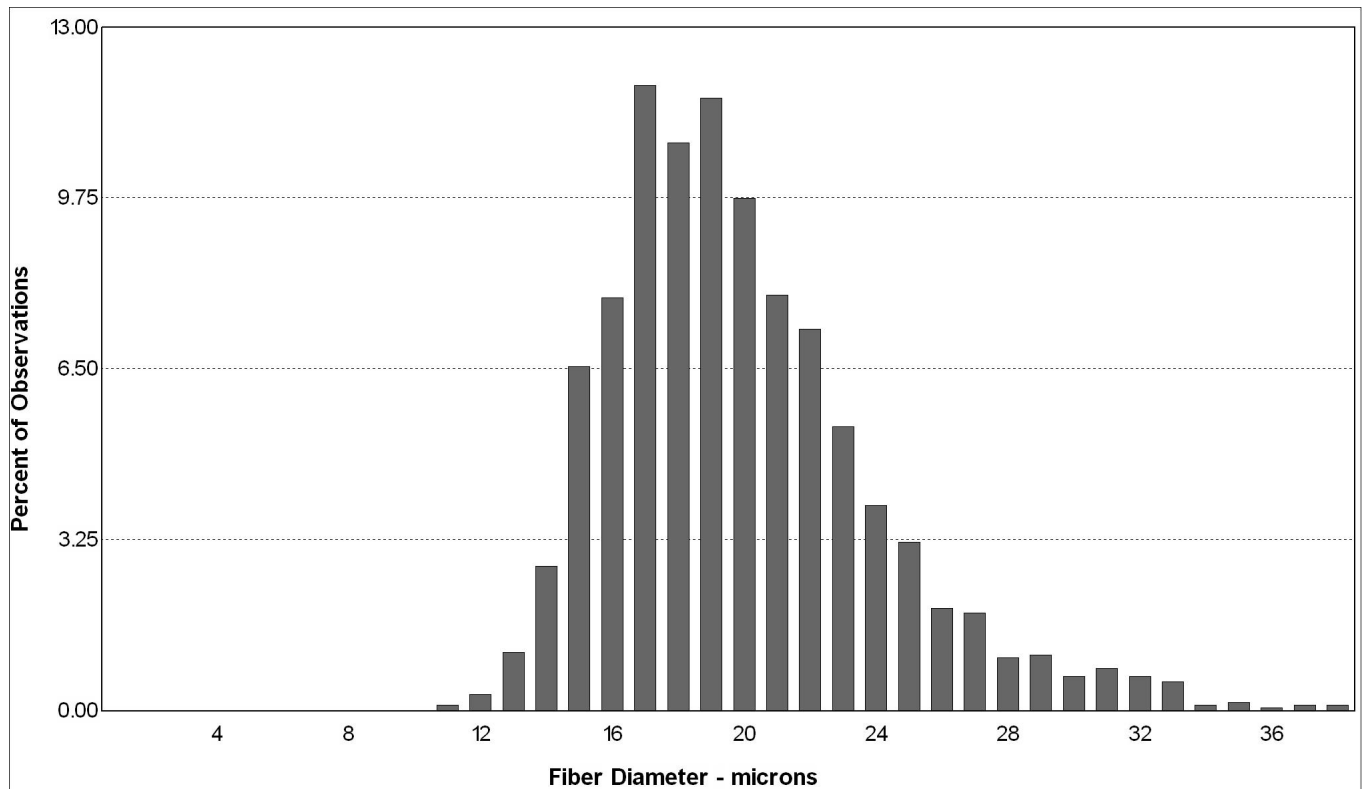

This Test Performed According to I.W.T.O Method 12