



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Borgstein Alpaca Farm/Karen Borgstein  
86 Plain St  
Medfield MA 02052-3303 USA

07/13/16

Test No: 926050


### Animal and Sample Description

**Animal Name:** Clemente  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** Med Fawn

**Animal ID:** 32387148  
**Sample Location:** Side  
**Sample Date:** 05/20/16  
**Age:** 08/15/14

### Laboratory Data

<b>Mean Fiber Diameter:</b>	20.2 microns	<b>Spin Fineness:</b>	19.8 microns
<b>Standard Deviation:</b>	4.4 microns	<b>Mean Curvature (deg/mm):</b>	44.8
<b>Coefficient of Variation:</b>	21.9 %	<b>SD Curvature (deg/mm):</b>	23.5
<b>Fibers Greater Than 30 microns:</b>	3.8 %	<b>Comfort Factor:</b>	96.2 %

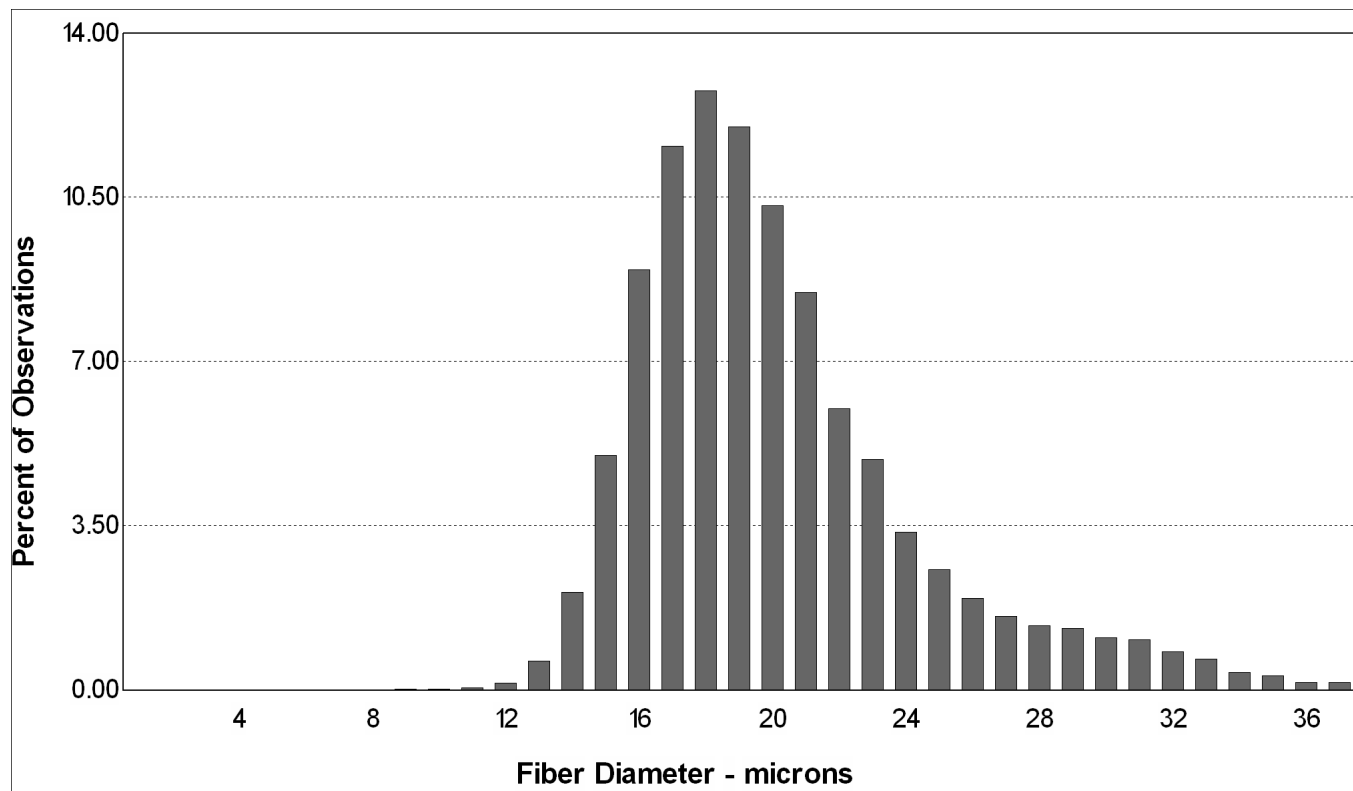

This Test Performed According to I.W.T.O Method 47