



**Yocom-McColl Testing Laboratories, Inc.**  
 540 West Elk Place • Denver, Colorado 80216-1823 USA  
 PHONE (303) 294-0582 • FAX (303) 295-6944  
 EMAIL: ymccoll@ymccoll.com

**Optical Fiber Diameter Analyser (OFDA100)  
 Micron Test Report**

Hubbert Farms/Kathy McConnell  
 600 Lily Lake Road  
 Peterborough OT K9J 0X3 Canada

09/09/10


Test No: 391006

**Animal and Sample Description**

Animal Name: Excelerator of Peterboro      Animal ID: 39296  
 Breed: Alpaca(Huacaya)      Sample Location: Blanket  
 Sex: Male      Sample Date: 05/15/10  
 Color: XXXXX      Age: 07/08/09

**Laboratory Data**

Mean Fiber Diameter: 18.3 microns      Spin Fineness: 17.7 microns  
 Standard Deviation: 3.7 microns      Mean Curvature (deg/mm): 34.9  
 Coefficient of Variation: 20.4 %      SD Curvature (deg/mm): 23.1  
 Fibers Greater Than 30 microns: 0.7 %      Comfort Factor: 99.3 %  
 Medullated Fibers: 9.4 %

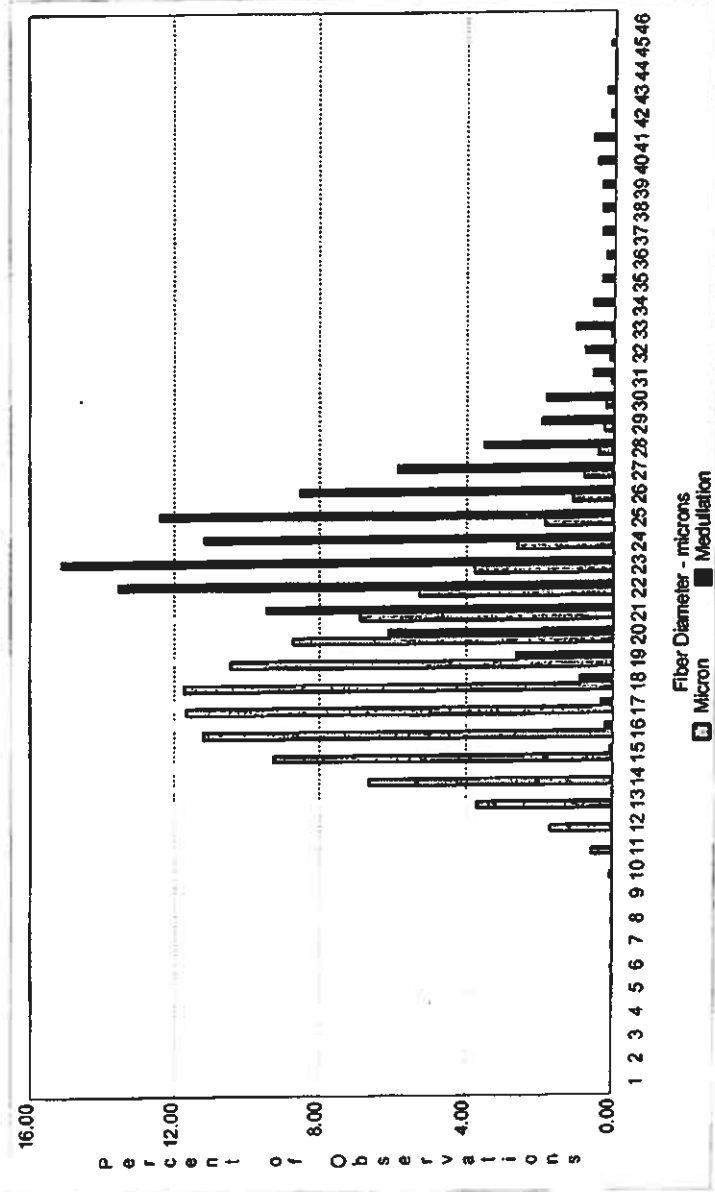

This Test Performed According to I.W.T.O Method 47