



Yocom-McColl Testing Laboratories, Inc.
540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100)
Micron Test Report

Hubbert Farms/Kathy McConnell
600 Lily Lake Rd
Peterborough ON K9J 6X3 Canada

09/29/11

Test No: 419558


Animal and Sample Description

Animal Name: MLT Cocoa Miss
Breed: Alpaca(Huacaya)
Sex: Female
Color: Brown

Animal ID: 30889101
Sample Location: Blanket
Sample Date: 05/10/11
Age: 05/28/07

Laboratory Data

Mean Fiber Diameter:	20.3 microns	Spin Fineness:	19.4 microns
Standard Deviation:	3.8 microns	Mean Curvature (deg/mm):	50.9
Coefficient of Variation:	18.9 %	SD Curvature (deg/mm):	28.8
Fibers Greater Than 30 microns:	1.7 %	Comfort Factor:	98.3 %

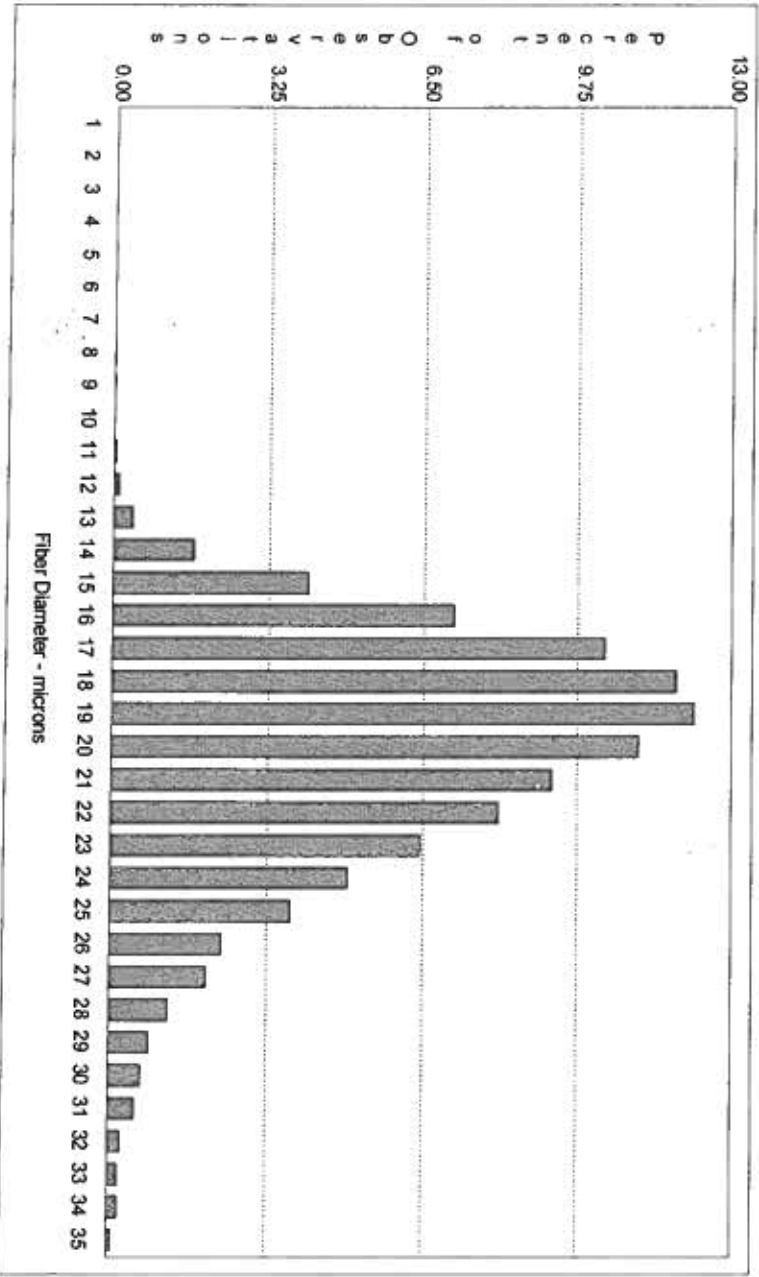

This Test Performed According to I.W.T.O Method 47