



Yocom-McColl Testing Laboratories, Inc.
540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100)
Micron Test Report

Hubbert Farms/Kathy McConnell
600 Lily Lake Rd
Peterborough ON K9J 6X3 Canada

09/29/11

Test No: 419557


Animal and Sample Description

Animal Name: Sunny Hill's Crystal White
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: 31158749
Sample Location: Blanket
Sample Date: 05/10/11
Age: 06/12/10

Laboratory Data

Mean Fiber Diameter:	20.1 microns	Spin Fineness:	19.9 microns
Standard Deviation:	4.6 microns	Mean Curvature (deg/mm):	44.5
Coefficient of Variation:	23.1 %	SD Curvature (deg/mm):	27.9
Fibers Greater Than 30 microns:	3.2 %	Comfort Factor:	96.8 %
Medullated Fibers:	7.2 %		

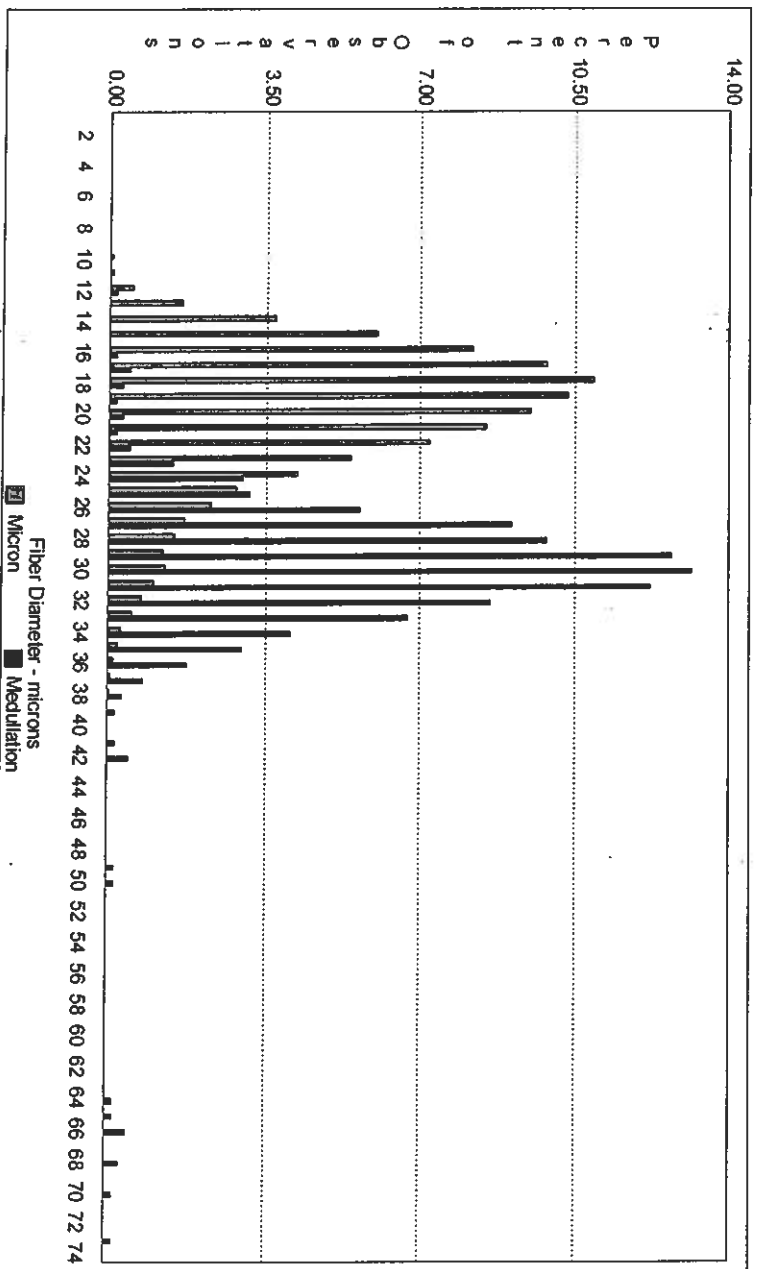

This Test Performed According to I.W.T.O Method 47