



Yocom-McColl Testing Laboratories, Inc.
540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100)
Micron Test Report

Hubbert Farms/Kathy McConnell
600 Lily Lake Road
Peterborough ON K9J 0X3 Canada

09/09/10


Test No: 391002

Animal and Sample Description

Animal Name:	Tell Libery	Animal ID:	30487
Breed:	Alpaca(Huacaya)	Sample Location:	Blanket
Sex:	Male	Sample Date:	05/15/10
Color:	White	Age:	05/05/05

Laboratory Data

Mean Fiber Diameter:	26.1 microns	Spin Fineness:	25.3 microns
Standard Deviation:	5.4 microns	Mean Curvature (deg/mm):	33.0
Coefficient of Variation:	20.7 %	SD Curvature (deg/mm):	21.0
Fibers Greater Than 30 microns:	17.8 %	Comfort Factor:	82.2 %
Medullated Fibers:	51.6 %		

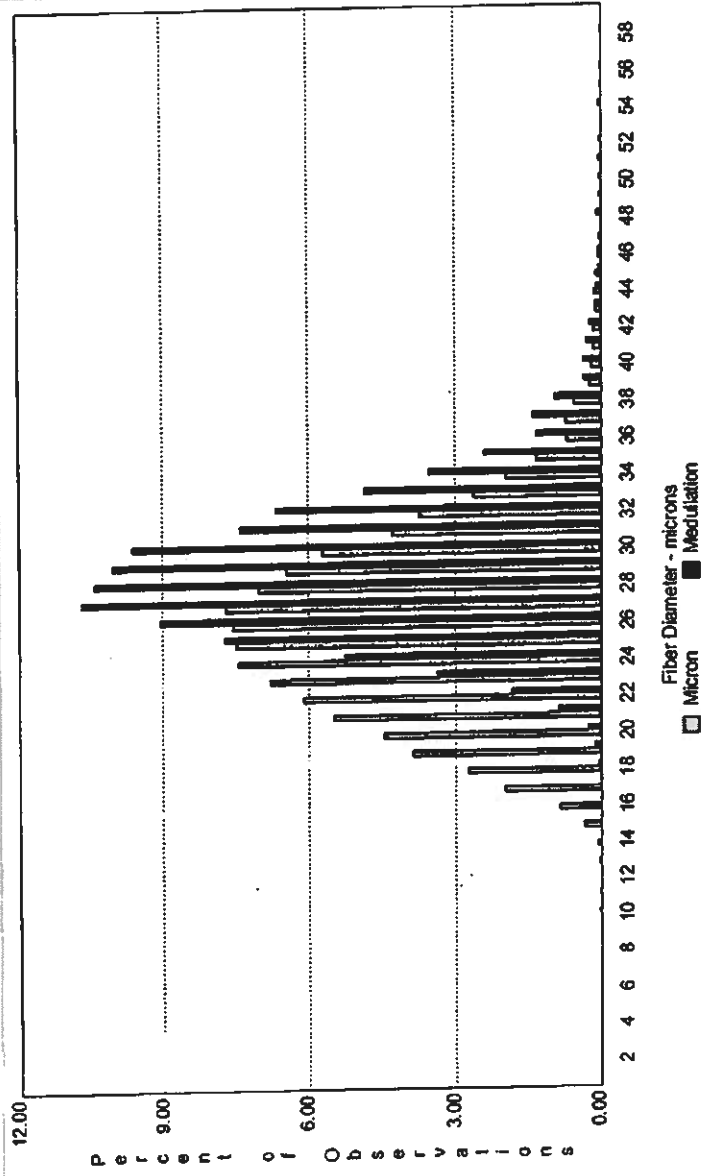

This Test Performed According to I.W.T.O Method 47