



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Aussie Hill Alpacas, Inc./Mary Blowers
4975 South Hill Rd
Canandaigua NY 14424 USA

09/02/09

Test No: 362088


Animal and Sample Description

Animal Name: Checkmate
Breed: Alpaca(Huacaya)
Sex: XXXXX
Color: XXXXX

Animal ID: XXXXX
Sample Location: Side
Sample Date: XX/XX/XX
Age: 09/05/08

Laboratory Data

Mean Fiber Diameter: 17.2 microns
Standard Deviation: 3.0 microns
Coefficient of Variation: 17.3 %
Fibers Greater Than 30 microns: 0.5 %

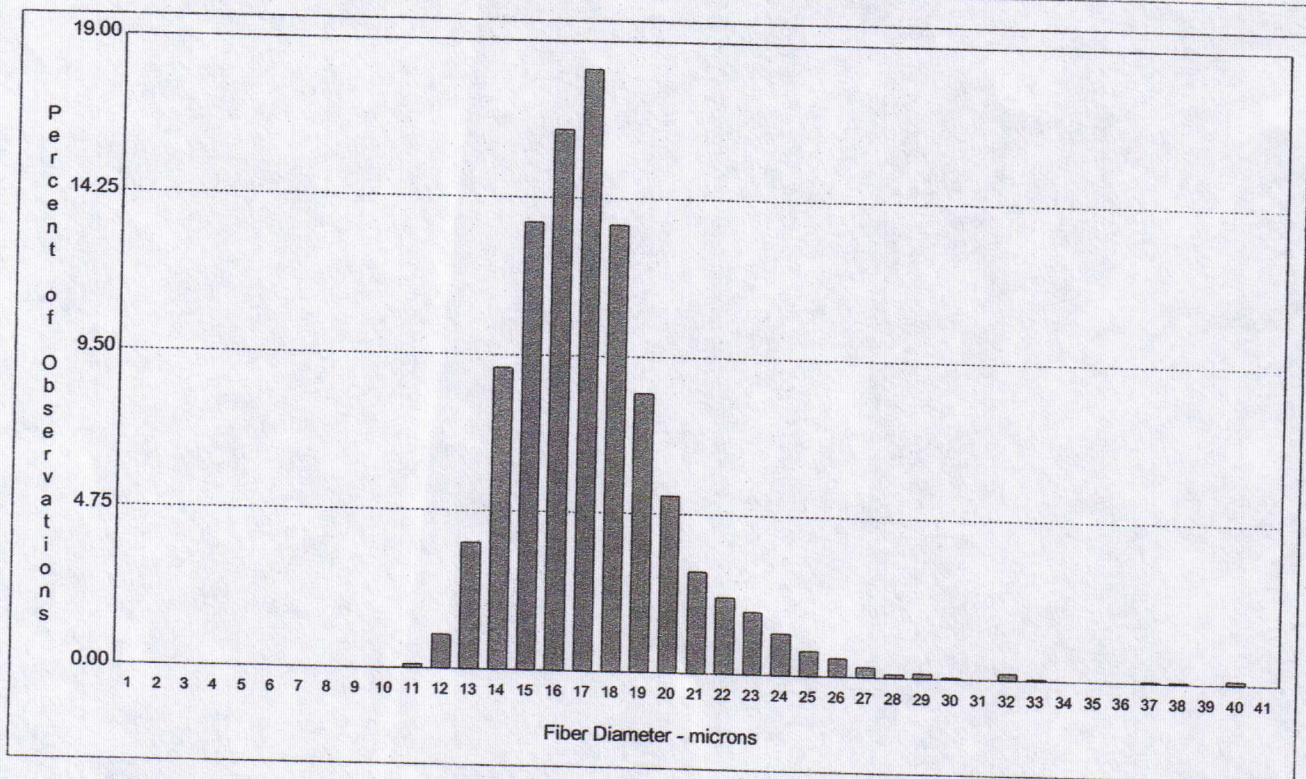

This Test Performed According to I.W.T.O Method 12