



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Pleasant Prairie Suris/Verna Carpenter
4101 N Ashton Road
Otis Orchard WA 99027 USA

Date: 07/18/16

Test No: 928209


Animal and Sample Description

Animal Name: Sansa of PPS
Breed: Alpaca(Suri)
Sex: Female
Color: Med Fawn

Animal ID: 35303671
Sample Location: Side
Sample Date: 06/04/16
Age: 05/28/15

Laboratory Data

Mean Fiber Diameter:	20.6 microns	Fibers Greater Than 30 microns:	4.4 %
Standard Deviation:	5.4 microns	Comfort Factor:	95.6 %
Coefficient of Variation:	26.4 %	Mean Curvature:	15.6 deg/mm
Spin Fineness:	21.0 microns	SD Curvature:	20.4 deg/mm

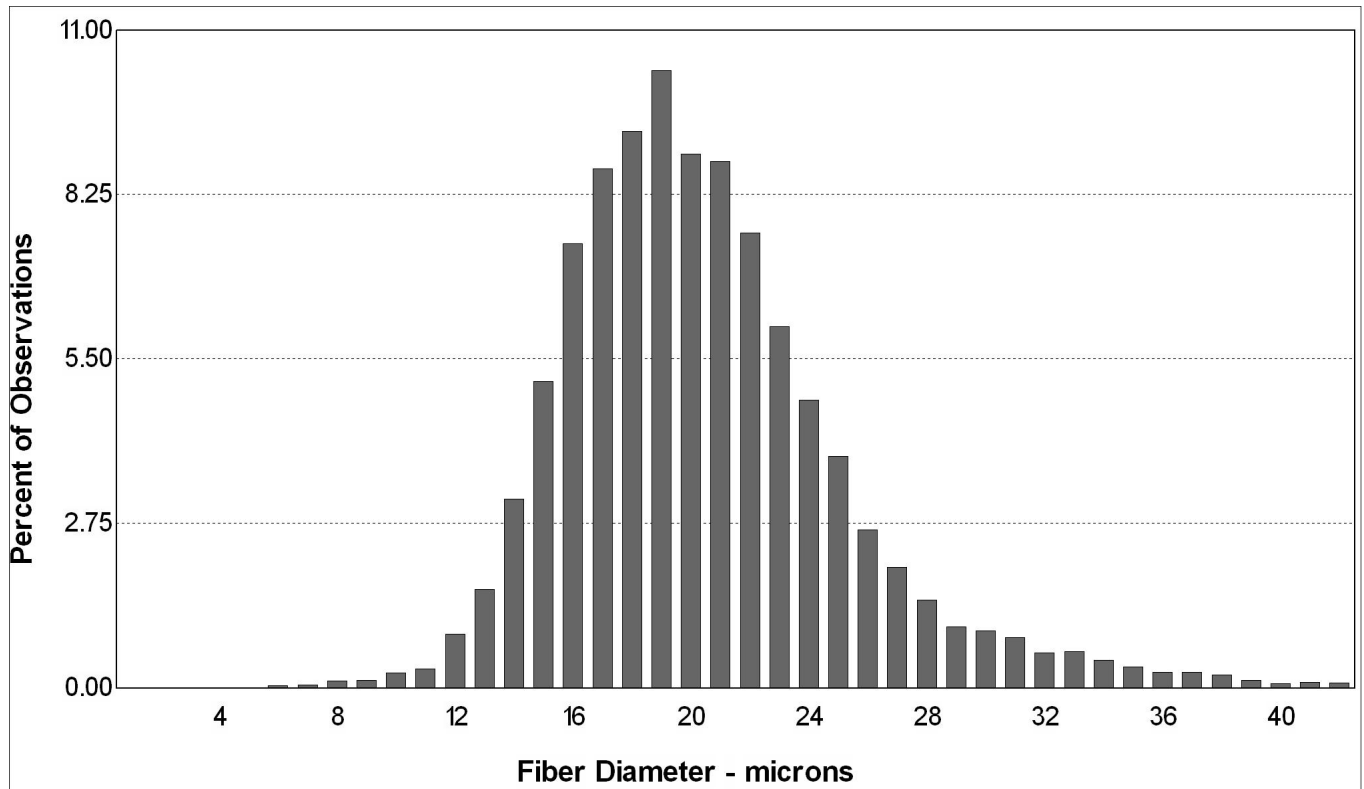

This Test Performed According to I.W.T.O Method 47