



Yocom-McColl Testing Laboratories, Inc.
540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

**Sirolan Laserscan
Micron Test Report**

Painted Sky Alpaca Farm/Mitchell Dickinson
95 Knight House Lane
Earleville MD 21919 USA

12/11/13

Test No: 473433


Animal and Sample Description

Animal Name: Ziva of Crimphaven
Breed: Alpaca(Huacaya)
Sex: Female
Color: Lt Brown

Animal ID: 32282771
Sample Location: Side (R)
Sample Date: 04/18/13
Age: 10/16/12

Laboratory Data

Mean Fiber Diameter: 20.4 microns
Standard Deviation: 4.6 microns
Coefficient of Variation: 22.4 %
Fibers Greater Than 30 microns: 1.9 %

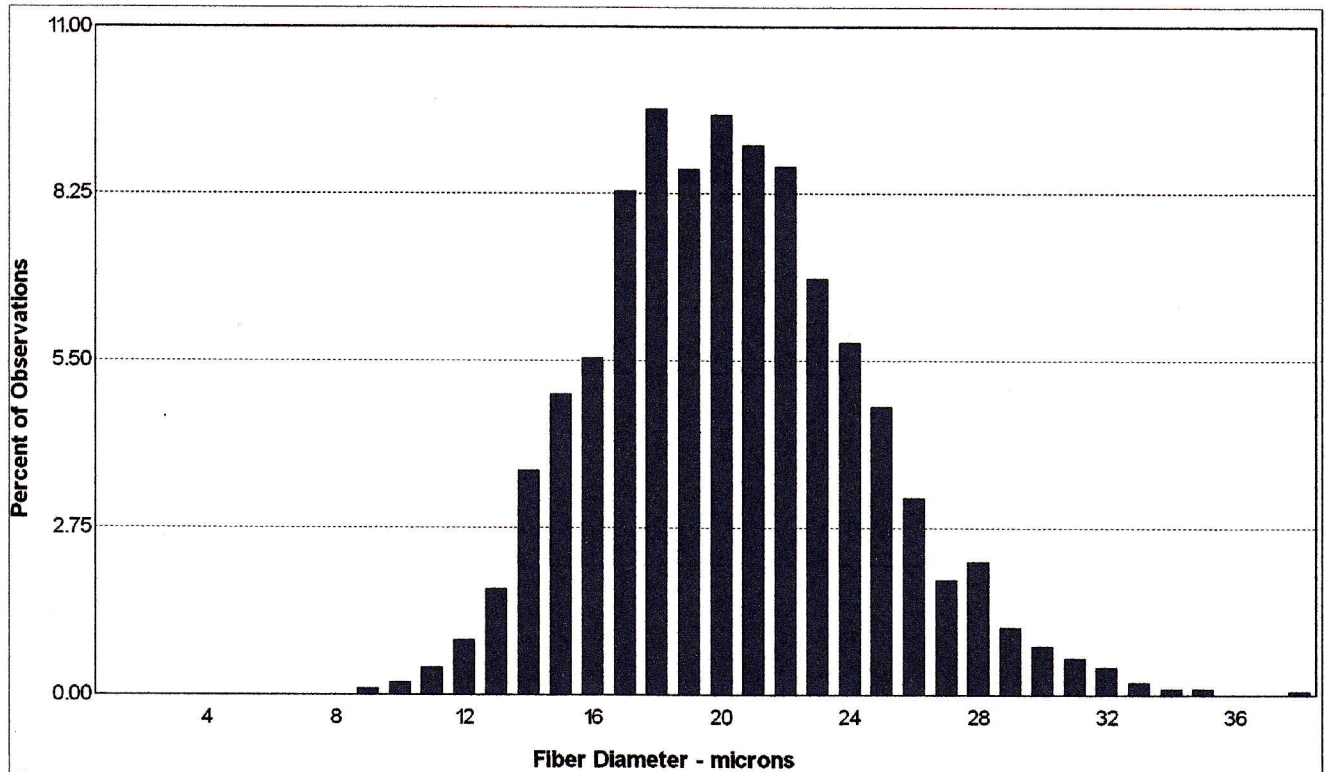

This Test Performed According to I.W.T.O Method 12