

# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Alpaca Harmony, LLC/Brandy Henson  
1453 Talmaks Rd  
Craigmont ID 83523-5015 USA

**Date:** 08/30/12  
**IAC No:** 28323  
**Test No:** 440622


### Animal and Sample Description

**Animal Name:** Earth Angel of Aharmony  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Med Fawn

**Animal ID:** 32761733  
**Sample Location:** Side  
**Sample Date:** 06/05/12  
**Age:** 07/25/11

### Laboratory Data

<b>Mean Fiber Diameter:</b>	20.2 microns	<b>Fibers Greater Than 30 microns:</b>	3.7 %
<b>Standard Deviation:</b>	4.8 microns	<b>Comfort Factor:</b>	96.3 %
<b>Coefficient of Variation:</b>	23.8 %	<b>Mean Curvature:</b>	32.6 deg/mm
<b>Spin Fineness:</b>	20.2 microns	<b>SD Curvature:</b>	22.7 deg/mm

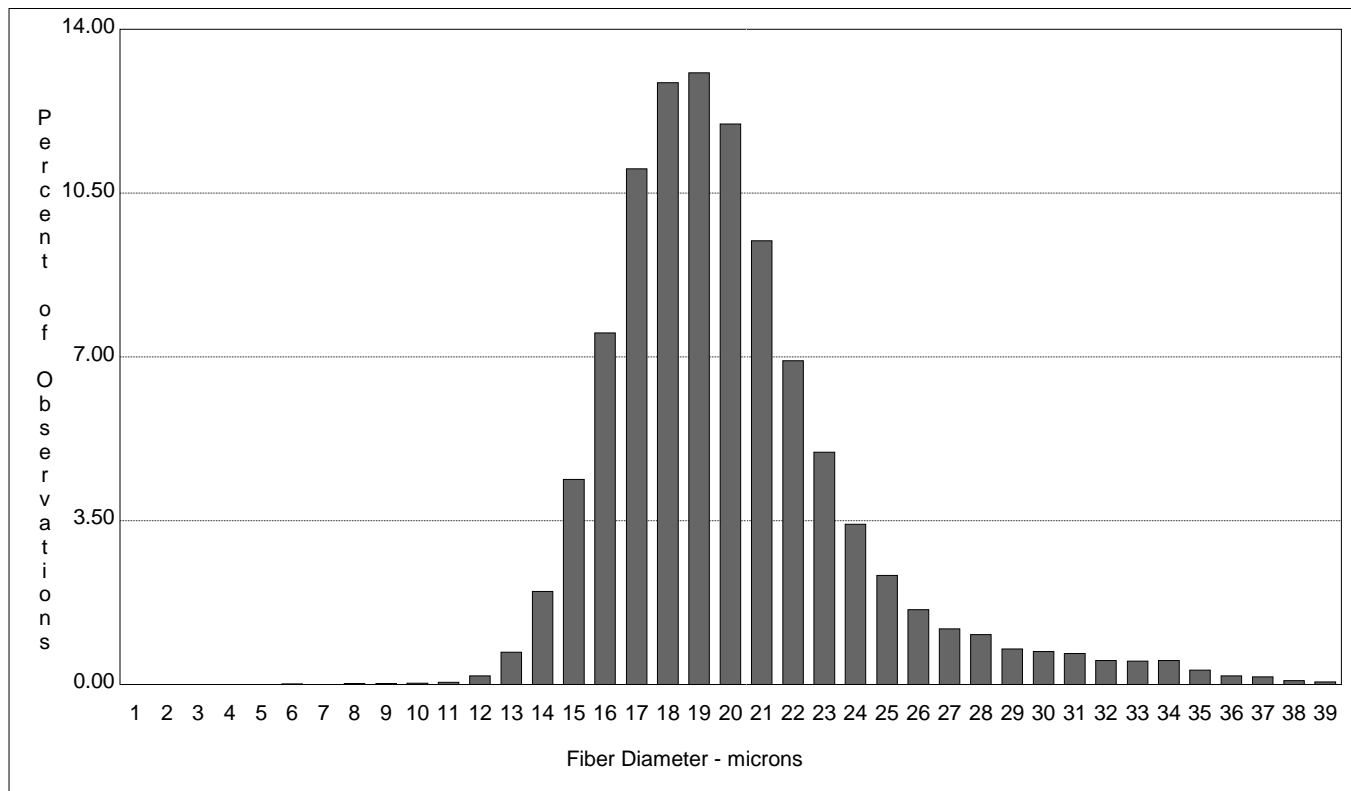

This Test Performed According to I.W.T.O Method 47