



Yocom-McColl Testing Laboratories, Inc.
540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

**Sirolan Laserscan
Micron Test Report**

Faith and Fleece Alpacas/Tracy Pellegrino
2664 N Mountain Ave.
Upland CA 91784 USA

09/04/14

Test No: 492289


Animal and Sample Description

Animal Name: Greystone's Aftershock
Breed: Alpaca(Suri)
Sex: Male
Color: Rose Grey

Animal ID: 32752984
Sample Location: Mid Side
Sample Date: 08/19/14
Age: 05/22/12

Laboratory Data

Mean Fiber Diameter: 25.8 microns
Standard Deviation: 5.7 microns
Coefficient of Variation: 22.2 %
Fibers Greater Than 30 microns: 17.4 %

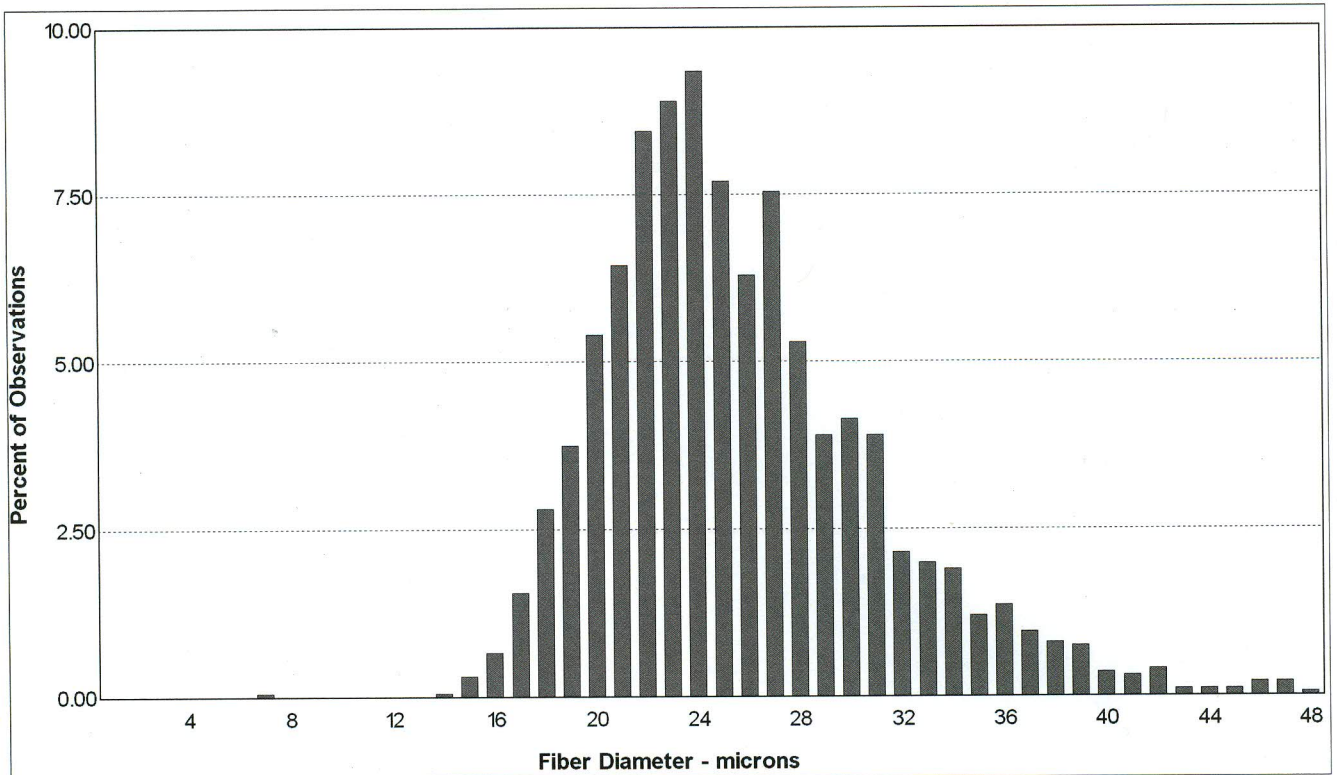

This Test Performed According to I.W.T.O Method 12