



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Shiloh Springs Ranch/Nancy Masak  
39505 Avenida Bonita  
Murrieta CA 92562

04/27/17

Test No: 940935


### Animal and Sample Description

**Animal Name:** Our Shiloh's Ilaria  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** MSG

**Animal ID:** 35162094  
**Sample Location:** Side (L)  
**Sample Date:** 04/07/17  
**Age:** 10/31/16

### Laboratory Data

**Mean Fiber Diameter:** 19.5 microns  
**Standard Deviation:** 4.2 microns  
**Coefficient of Variation:** 21.5 %  
**Fibers Greater Than 30 microns:** 2.2 %

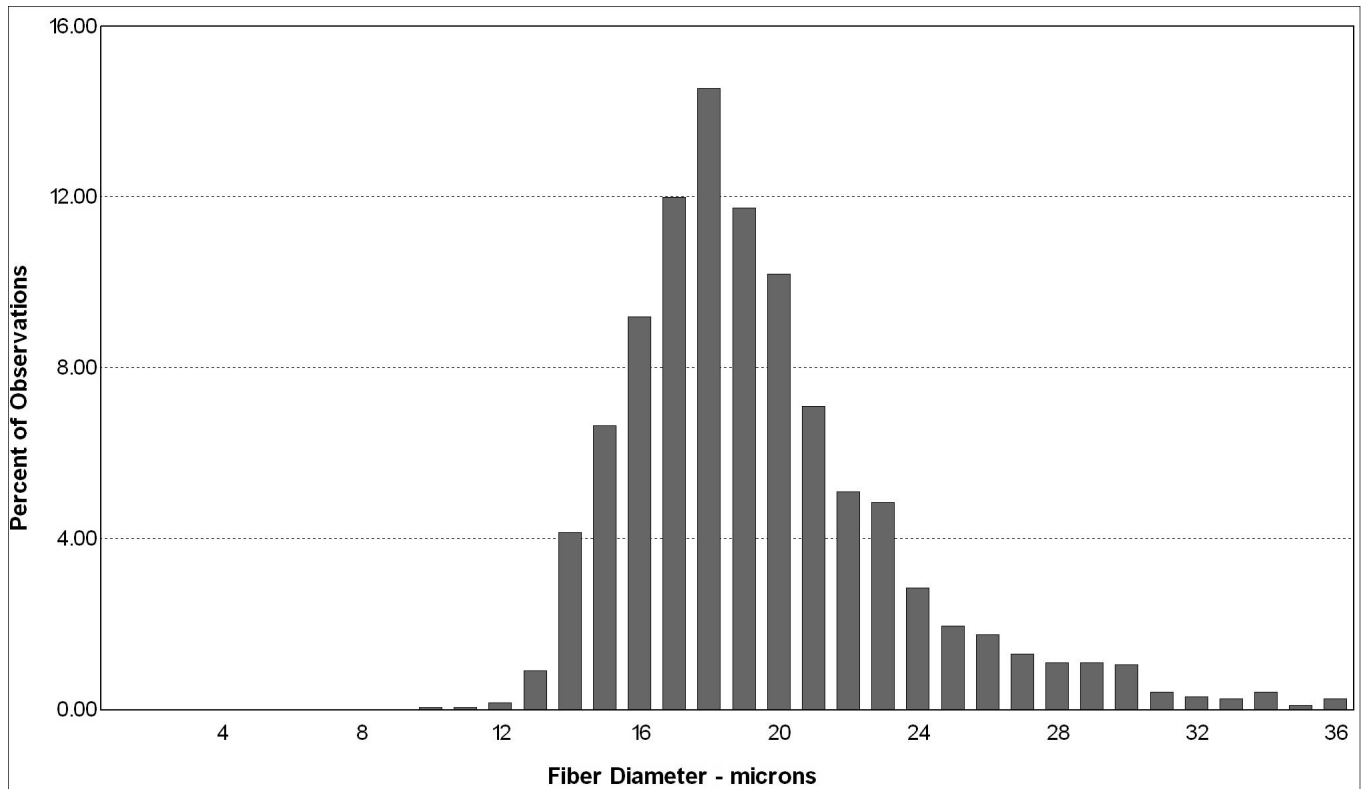

This Test Performed According to I.W.T.O Method 12