



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Alpagas Fibrefine/Karine Tremblay/Emanuel Caron  
714 rang des Érables  
Sainte-Eulalie QC G0Z 1E0 Canada

06/26/18

Test No: 962200


### Animal and Sample Description

**Animal Name:** Fibrefine Lana Kane  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** White

**Animal ID:** 32665611  
**Sample Location:** Side  
**Sample Date:** 04/30/18  
**Age:** 11/07/16

### Laboratory Data

<b>Mean Fiber Diameter:</b>	16.1 microns	<b>Spin Fineness:</b>	15.5 microns
<b>Standard Deviation:</b>	3.2 microns	<b>Mean Curvature (deg/mm):</b>	45.1
<b>Coefficient of Variation:</b>	19.5 %	<b>SD Curvature (deg/mm):</b>	28.8
<b>Fibers Greater Than 30 microns:</b>	0.2 %	<b>Comfort Factor:</b>	99.8 %

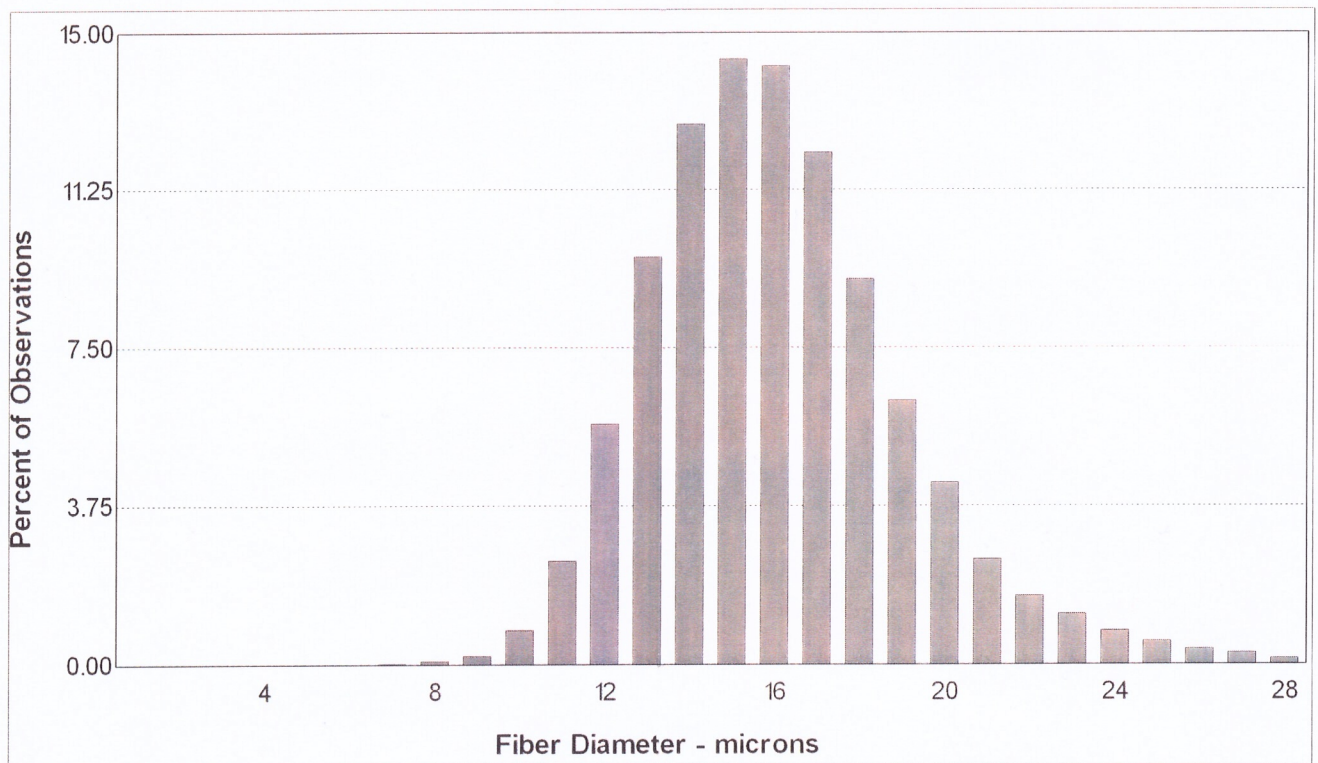

This Test Performed According to I.W.T.O Method 47