



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Gates Alpaca Ranch/Andrew & Kristina Gates  
48531 Russia Road  
Amherst OH 44001 USA


**Date:** 07/22/17  
**Shear ID:** 144077  
**Test No:** 945622

### Animal and Sample Description

<b>Animal Name:</b>	G8S Realto's Peruvian Hershey	<b>Date of Birth (Age):</b>	06/08/16
<b>ARI #:</b>	32459739	<b>Sample Location:</b>	Side
<b>Breed:</b>	Alpaca(Huacaya)	<b>Sample Date:</b>	05/16/17
<b>Sex:</b>	Male	<b>Previous Shear Date:</b>	06/18/16
<b>Color:</b>	Med Fawn	<b>Total Fleece Wt (lbs):</b>	4.40

### Laboratory Data

<b>Mean Fiber Diameter:</b>	19.6 microns	<b>Mean Staple Length:</b>	102.2 mm
<b>Standard Deviation:</b>	3.8 microns	<b>Length Standard Deviation:</b>	4.9 mm
<b>Coefficient of Variation:</b>	19.6 %	<b>Length Coefficient of Variation:</b>	4.8 %
<b>Spin Fineness:</b>	18.8 microns	<b>Mean Curvature:</b>	43.9 deg/mm
<b>Fibers Greater Than 30 microns:</b>	1.0 %	<b>SD Curvature:</b>	23.9 deg/mm
<b>Comfort Factor:</b>	99.0 %		

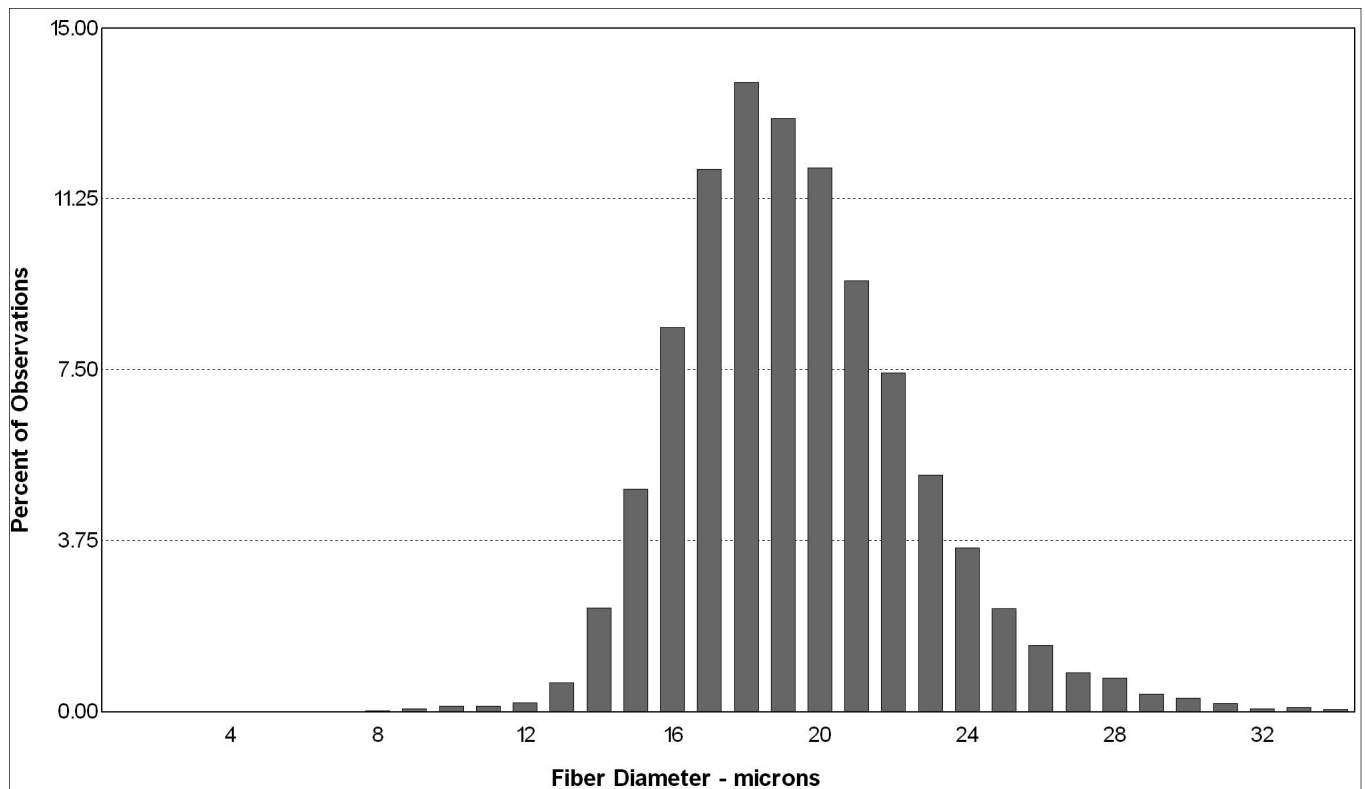

This Test Performed According to I.W.T.O Method 47