



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Andean Group/Glengary Farm/Patrick Cassese  
2704 Slessman Drive  
Plymouth OH 44865 USA

07/16/15

Test No: 906712


### Animal and Sample Description

**Animal Name:** GGF Xeno's Priapus  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** Lt Fawn

**Animal ID:** 35210528  
**Sample Location:** Side  
**Sample Date:** 05/15/15  
**Age:** 09/14/14

### Laboratory Data

|                                        |              |                                 |              |
|----------------------------------------|--------------|---------------------------------|--------------|
| <b>Mean Fiber Diameter:</b>            | 17.4 microns | <b>Spin Fineness:</b>           | 18.1 microns |
| <b>Standard Deviation:</b>             | 4.9 microns  | <b>Mean Curvature (deg/mm):</b> | 37.7         |
| <b>Coefficient of Variation:</b>       | 27.9 %       | <b>SD Curvature (deg/mm):</b>   | 23.7         |
| <b>Fibers Greater Than 30 microns:</b> | 1.9 %        | <b>Comfort Factor:</b>          | 98.1 %       |

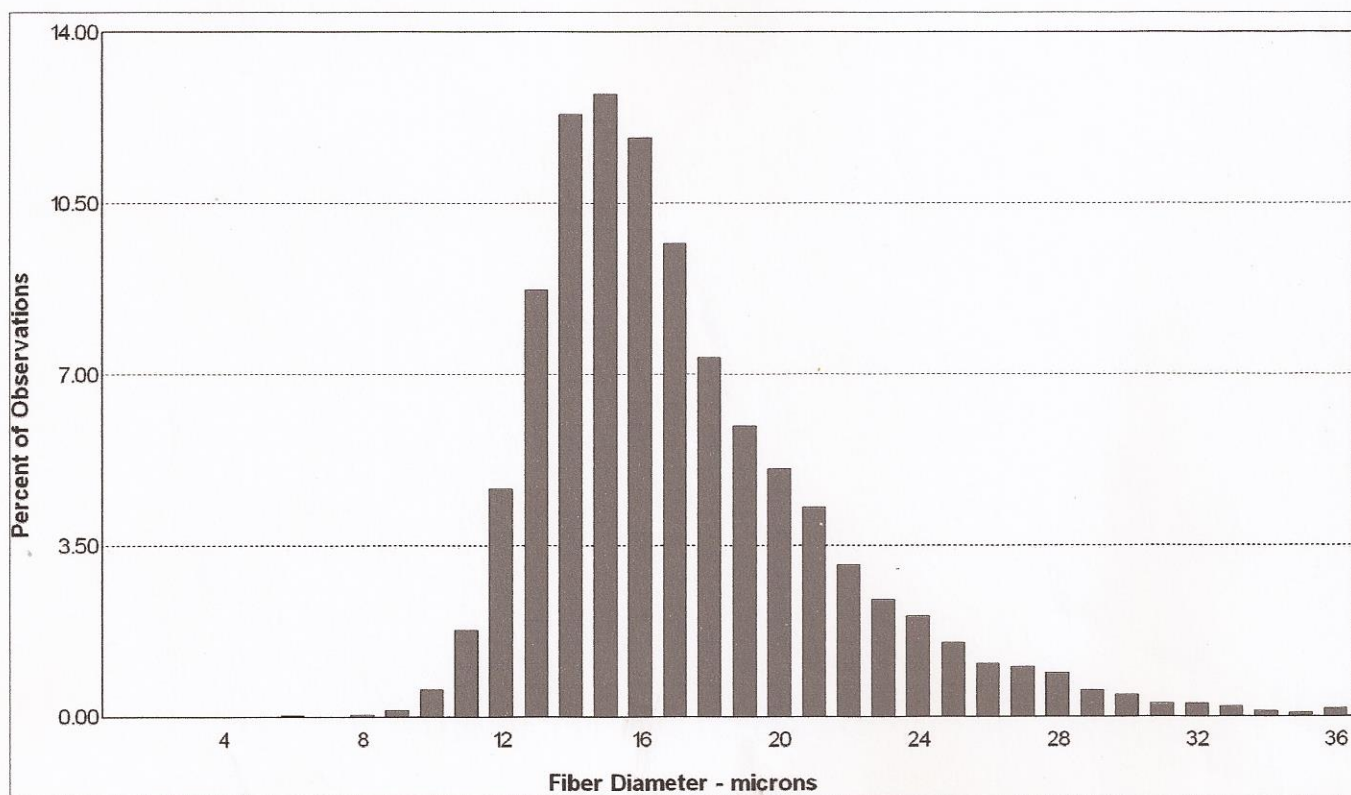

This Test Performed According to I.W.T.O Method 47