



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Flatland Ranch/Steve Trainer
21302 SW County Line Rd
Rose Hill KS 67133 USA

Date: 07/20/17

Test No: 945146


Animal and Sample Description

Animal Name: Storm Chaser
Breed: Alpaca(Huacaya)
Sex: Male
Color: Lt Fawn

Animal ID: 32628357
Sample Location: Side
Sample Date: 04/24/17
Age: 06/24/14

Laboratory Data

Mean Fiber Diameter:	17.8 microns	Fibers Greater Than 30 microns:	0.6 %
Standard Deviation:	4.0 microns	Comfort Factor:	99.4 %
Coefficient of Variation:	22.3 %	Mean Curvature:	44.9 deg/mm
Spin Fineness:	17.5 microns	SD Curvature:	24.8 deg/mm

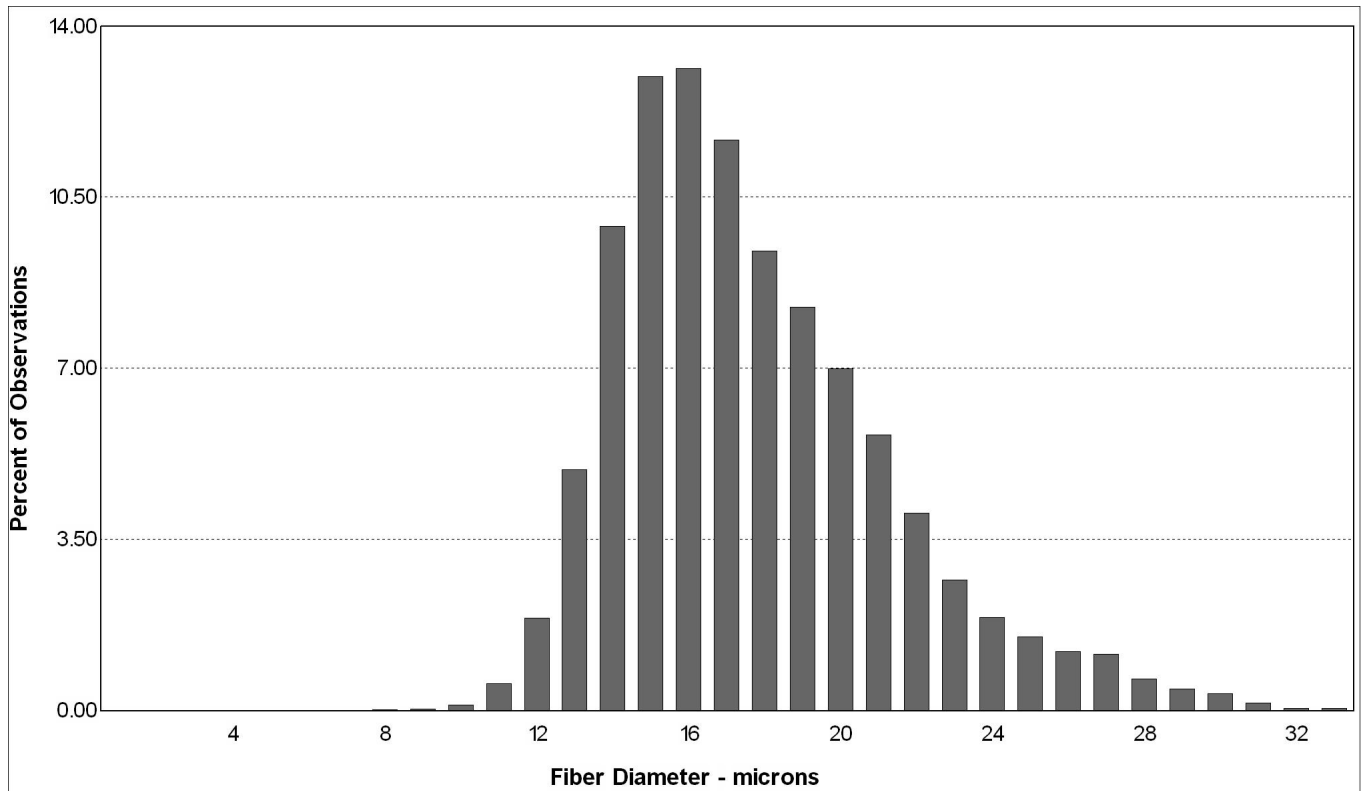

This Test Performed According to I.W.T.O Method 47