

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Delphi Alpacas/Linda Batt
P.O. Box 9
Coaldale CO 81222

06/14/11

Test No: 406219


Animal and Sample Description

Animal Name: Elyria
Breed: Alpaca(Huacaya)
Sex: Female
Color: Brown

Animal ID: XXXXX
Sample Location: Side
Sample Date: 05/09/11
Age: 08/23/10

Laboratory Data

Mean Fiber Diameter: 16.4 microns
Standard Deviation: 3.5 microns
Coefficient of Variation: 21.4 %
Fibers Greater Than 30 microns: 0.7 %

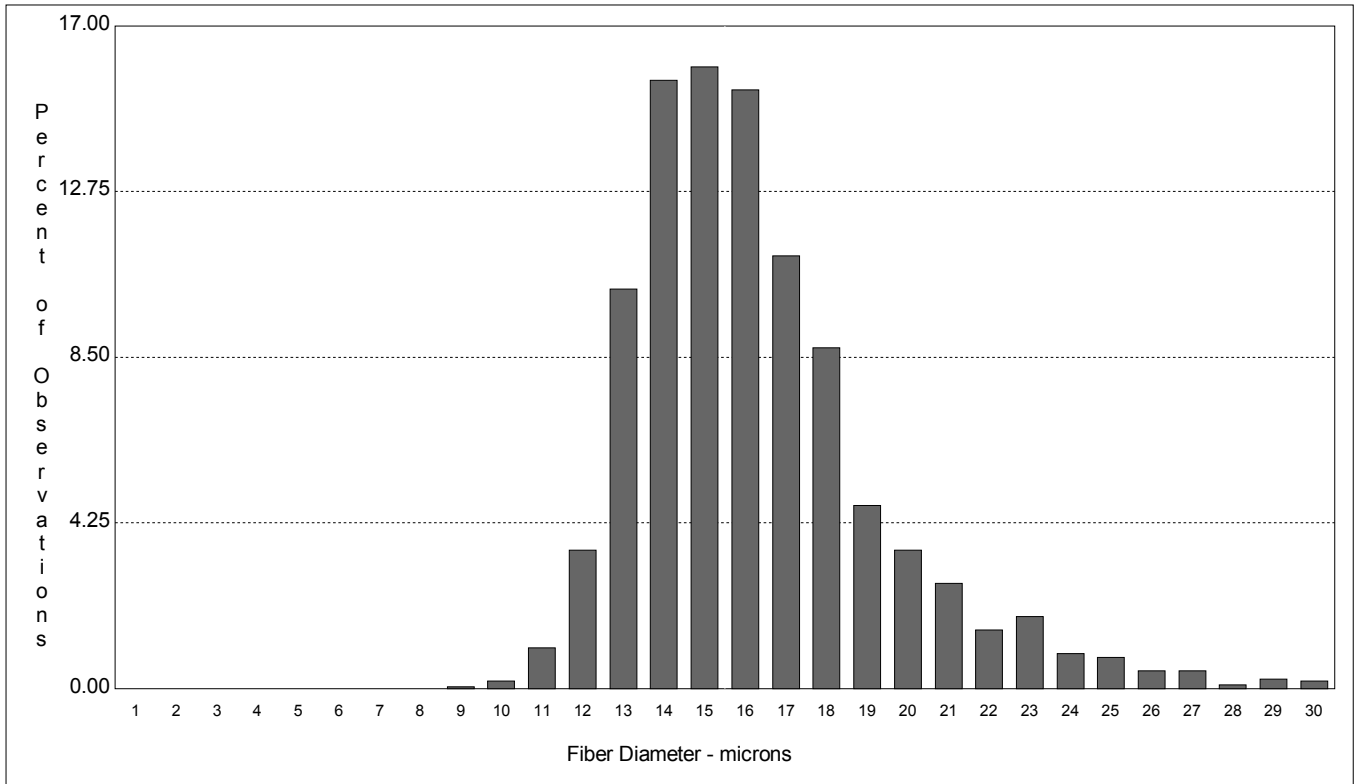

This Test Performed According to I.W.T.O Method 12