



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Squire Creek Ranch, LLC/Michael DeDear & Alan Pickard
41017 Squire Creek Rd
Arlington WA 98223 USA

07/28/14

Test No: 487184


Animal and Sample Description

Animal Name: Squire Creek's Nebraska
Breed: Alpaca(Huacaya)
Sex: Male
Color: Lt Rose Grey

Animal ID: 32242263
Sample Location: Side (R)
Sample Date: 05/31/14
Age: 07/28/11

Laboratory Data

Mean Fiber Diameter: 17.8 microns
Standard Deviation: 3.4 microns
Coefficient of Variation: 18.9 %
Fibers Greater Than 30 microns: 0.9 %

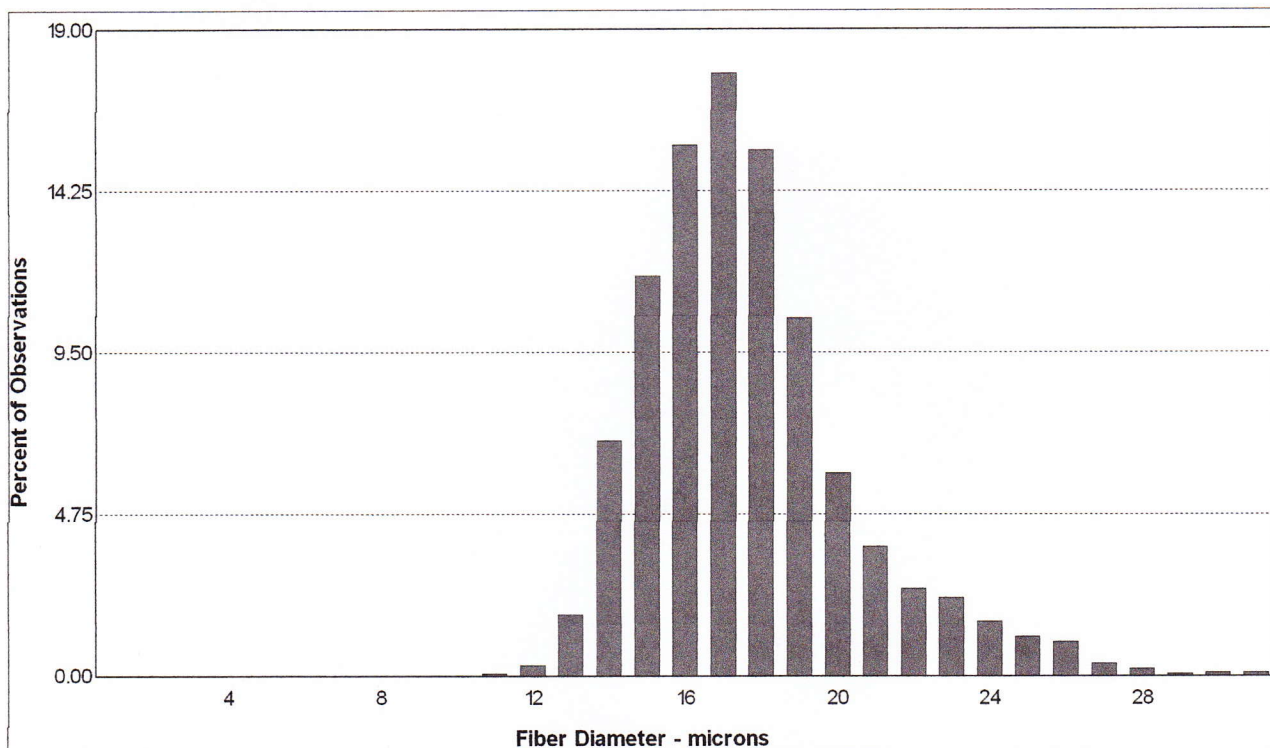

This Test Performed According to I.W.T.O Method 12