



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Three Niece Farm, LLC/Susan Beauregard
340 Providence Tpke, PO Box 163
Hampton CT 06247

07/15/13

Test No: 459777


Animal and Sample Description

Animal Name: Fiber Optic's Peruvian Princess
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: 30019776
Sample Location: Side (L)
Sample Date: 05/06/13
Age: 06/10/07

Laboratory Data

| | | | |
|--|--------------|---------------------------------|--------------|
| Mean Fiber Diameter: | 17.8 microns | Spin Fineness: | 17.1 microns |
| Standard Deviation: | 3.5 microns | Mean Curvature (deg/mm): | 55.8 |
| Coefficient of Variation: | 19.4 % | SD Curvature (deg/mm): | 29.4 |
| Fibers Greater Than 30 microns: | 0.6 % | Comfort Factor: | 99.4 % |

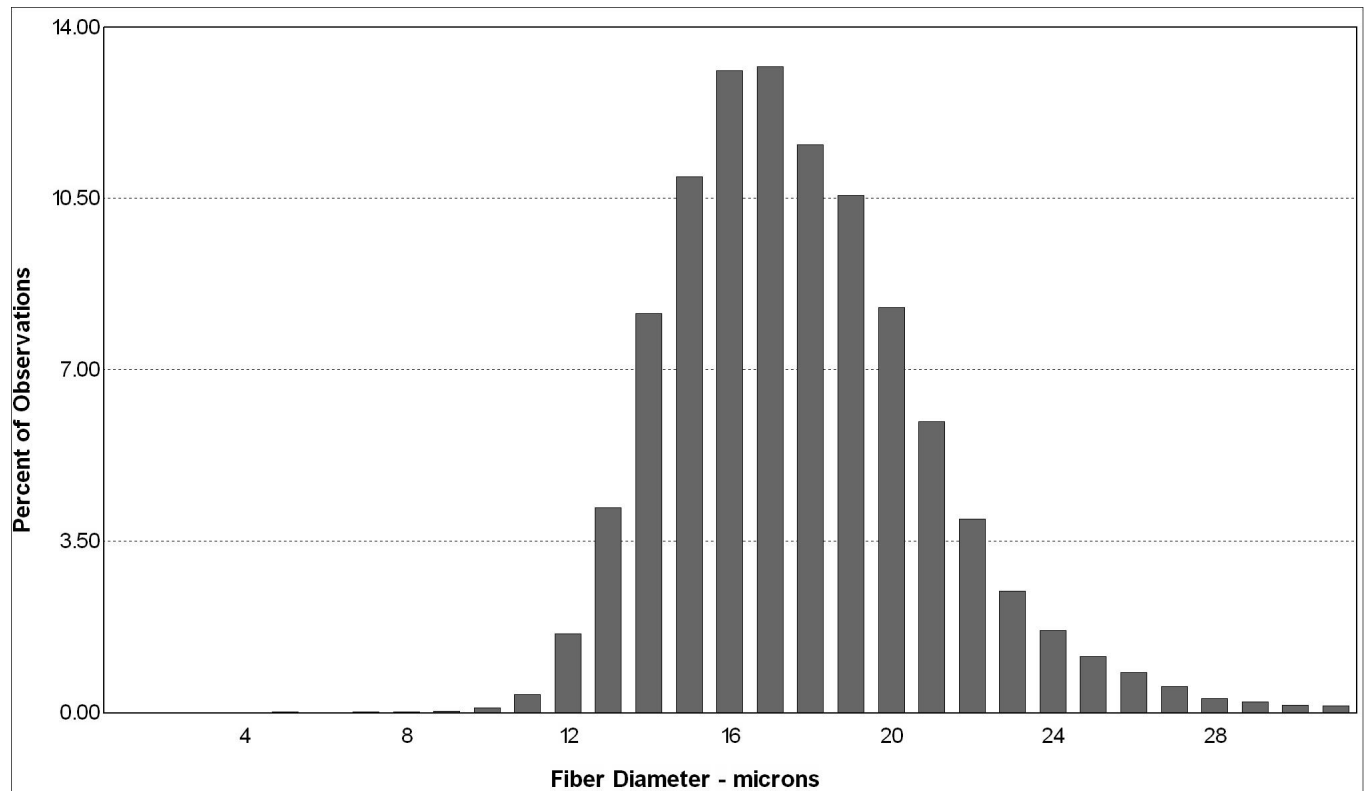

This Test Performed According to I.W.T.O Method 47