



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Thordarson Farms/Heather Thordarson
13492 S. Warnock Rd
Oregon City OR 97045 USA

Date: 07/27/16

Test No: 927874


Animal and Sample Description

Animal Name: Pearl of Persephone
Breed: Alpaca(Huacaya)
Sex: Female
Color: Lt Fawn

Animal ID: 35234388
Sample Location: Side
Sample Date: 06/06/16
Age: 07/20/14

Laboratory Data

Mean Fiber Diameter:	20.3 microns	Fibers Greater Than 30 microns:	3.2 %
Standard Deviation:	4.4 microns	Comfort Factor:	96.8 %
Coefficient of Variation:	21.9 %	Mean Curvature:	45.6 deg/mm
Spin Fineness:	19.9 microns	SD Curvature:	24.2 deg/mm

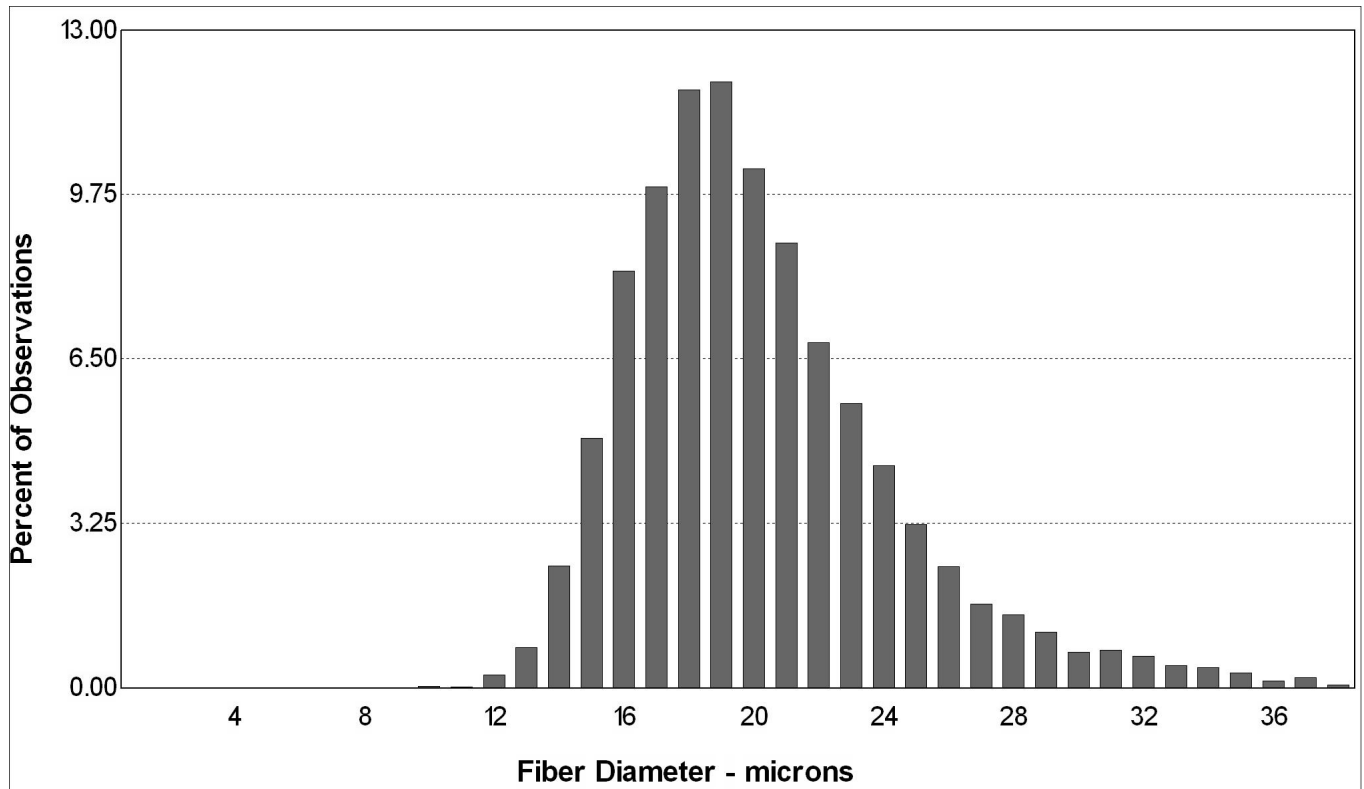

This Test Performed According to I.W.T.O Method 47