

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

R & R Ranch/Richard & Robin Vasquez
325B Denio Avenue
Gilroy CA 95020-9203 USA

07/19/10

Test No: 384138


Animal and Sample Description

Animal Name: Kaleidoscope
Breed: Alpaca(Huacaya)
Sex: Male
Color: Med Silver Grey

Animal ID: 31094856
Sample Location: Side
Sample Date: 06/03/10
Age: 06/27/07

Laboratory Data

Mean Fiber Diameter: 25.3 microns
Standard Deviation: 4.5 microns
Coefficient of Variation: 17.9 %
Fibers Greater Than 30 microns: 10.4 %

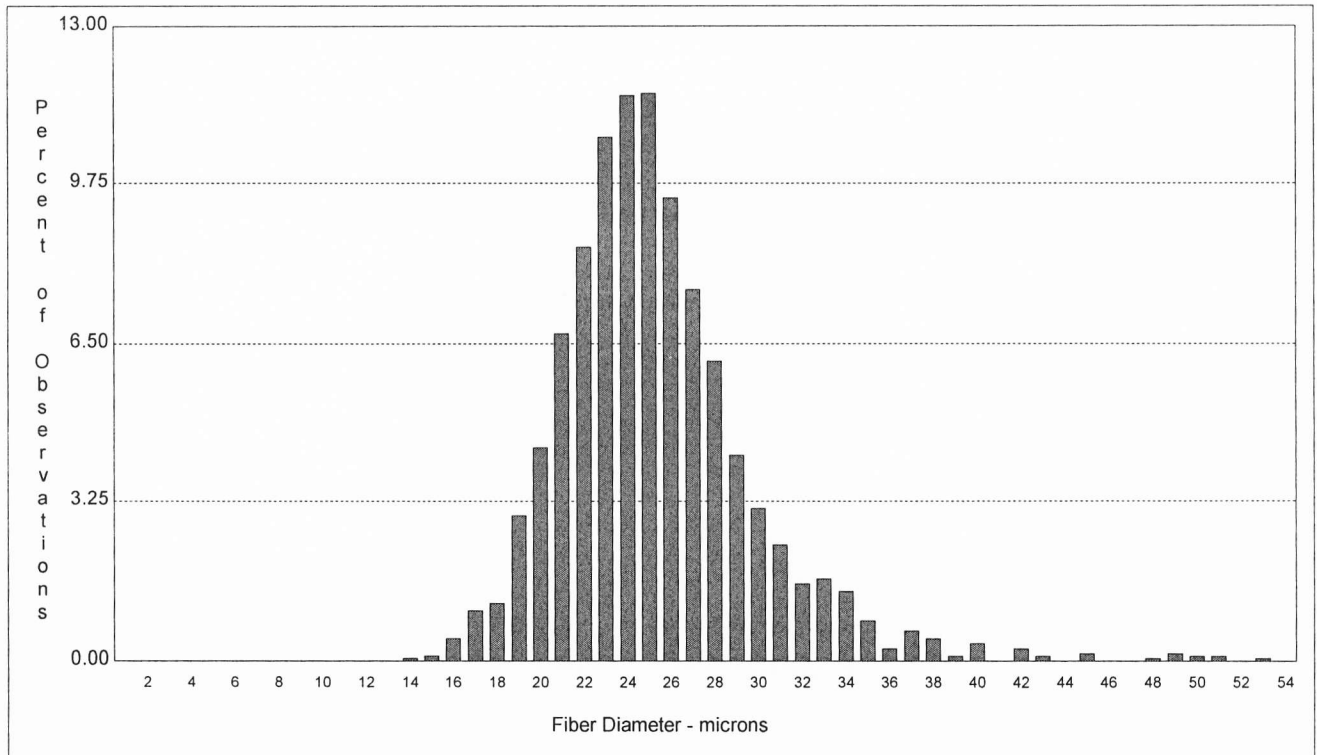

This Test Performed According to I.W.T.O Method 12