



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Alpaca Palace LLC/Renee A Ritenour  
102 Knotingham Lane  
Butler PA 16001

08/14/17


Test No: 942152

### Animal and Sample Description

<b>Animal Name:</b>	Alpaca Palace's Honeysuckle 027 625 519	<b>Animal ID:</b>	35110491
<b>Breed:</b>	Alpaca(Huacaya)	<b>Sample Location:</b>	Side (R)
<b>Sex:</b>	Female	<b>Sample Date:</b>	05/07/17
<b>Color:</b>	Beige	<b>Age:</b>	05/13/15

### Laboratory Data

<b>Mean Fiber Diameter:</b>	18.3 microns
<b>Standard Deviation:</b>	3.5 microns
<b>Coefficient of Variation:</b>	19.0 %
<b>Fibers Greater Than 30 microns:</b>	0.7 %

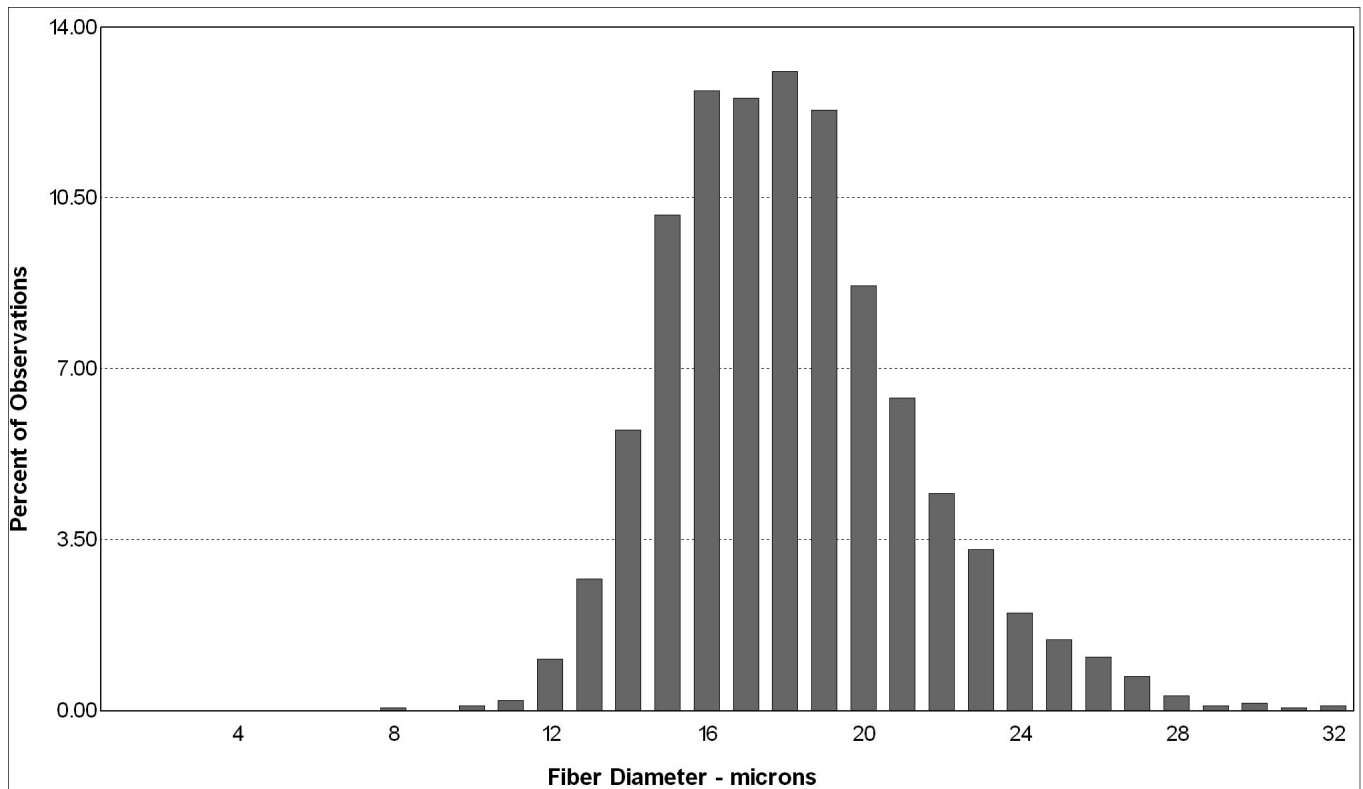

This Test Performed According to I.W.T.O Method 12