



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

West Penn Alpacas/Mike & Debbie Vigus
1843 E. Finley Dr
Claysville PA 15323 USA

Date: 06/01/16

Test No: 921356


Animal and Sample Description

Animal Name: Snowmass Legend Rising
Breed: Alpaca(Huacaya)
Sex: Male
Color: Beige

Animal ID: 32844030
Sample Location: Side (R)
Sample Date: 04/28/16
Age: 09/03/13

Laboratory Data

Mean Fiber Diameter:	19.6 microns	Fibers Greater Than 30 microns:	0.5 %
Standard Deviation:	3.2 microns	Comfort Factor:	99.5 %
Coefficient of Variation:	16.2 %	Mean Curvature:	47.4 deg/mm
Spin Fineness:	18.4 microns	SD Curvature:	23.6 deg/mm

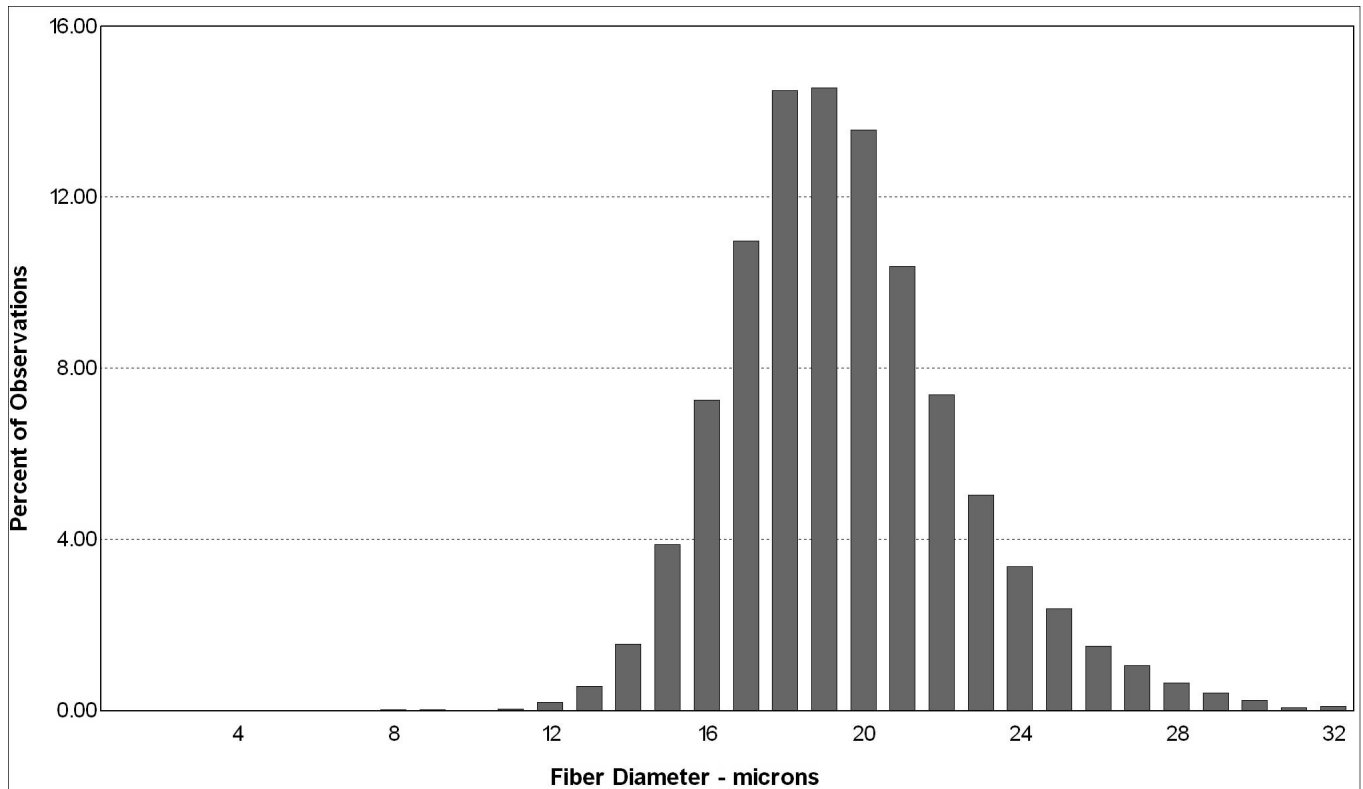

This Test Performed According to I.W.T.O Method 47