

Yocom-McColl Testing Laboratories, Inc.  
540 West Elk Place • Denver, Colorado 80216-1823 USA  
PHONE (303) 294-0582 • FAX (303) 295-6944  
EMAIL: ymccoll@ymccoll.com

**Sirolan Laserscan  
Micron Test Report**

Alpaca Palace LLC/Renee Ritenour  
102 Knotingham Lane  
Butler PA 16001

01/09/15


**Test No:** 496182

**Animal and Sample Description**

<b>Animal Name:</b>	Sunset Hills Zenterfold ET 57358368	<b>Animal ID:</b>	32423020
<b>Breed:</b>	Alpaca(Huacaya)	<b>Sample Location:</b>	Side (R)
<b>Sex:</b>	Female	<b>Sample Date:</b>	05/10/14
<b>Color:</b>	Lt Fawn	<b>Age:</b>	06/10/12

**Laboratory Data**

<b>Mean Fiber Diameter:</b>	17.6 microns
<b>Standard Deviation:</b>	3.7 microns
<b>Coefficient of Variation:</b>	21.0 %
<b>Fibers Greater Than 30 microns:</b>	1.0 %

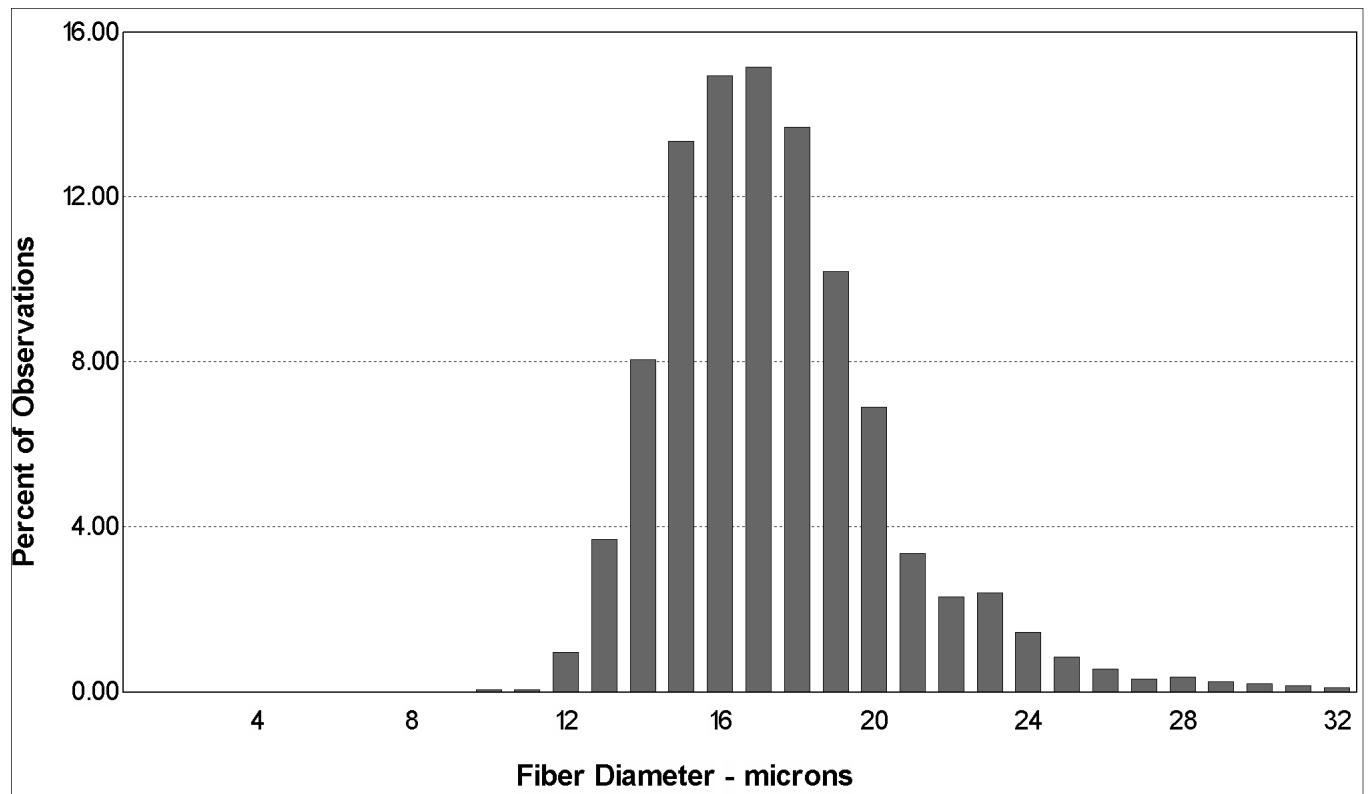

**This Test Performed According to I.W.T.O Method 12**