



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Snowmass Alpacas LLC/Lynn Edens  
270 Rapid Lightning Road  
Sandpoint ID 83864-4746 USA

**Date:** 10/31/17  
**Shear ID:** 159564  
**Test No:** 952958


### Animal and Sample Description

**Animal Name:** Snowmass Aqua Oasis XX  
**ARI #:** 35096139  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** White

**Date of Birth (Age):** 06/20/16  
**Sample Location:** Grid  
**Sample Date:** 05/10/17  
**Previous Shear Date:** XX/XX/XX  
**Total Fleece Wt (lbs):** 0.00

### Laboratory Data

<b>Mean Fiber Diameter:</b>	14.0 microns	<b>Mean Staple Length:</b>	111.4 mm
<b>Standard Deviation:</b>	3.7 microns	<b>Length Standard Deviation:</b>	9.5 mm
<b>Coefficient of Variation:</b>	26.7 %	<b>Length Coefficient of Variation:</b>	8.5 %
<b>Spin Fineness:</b>	14.3 microns	<b>Mean Curvature:</b>	64.3 deg/mm
<b>Fibers Greater Than 30 microns:</b>	0.6 %	<b>SD Curvature:</b>	35.2 deg/mm
<b>Comfort Factor:</b>	99.4 %	<b>Medullated Fibers:</b>	1.7 %

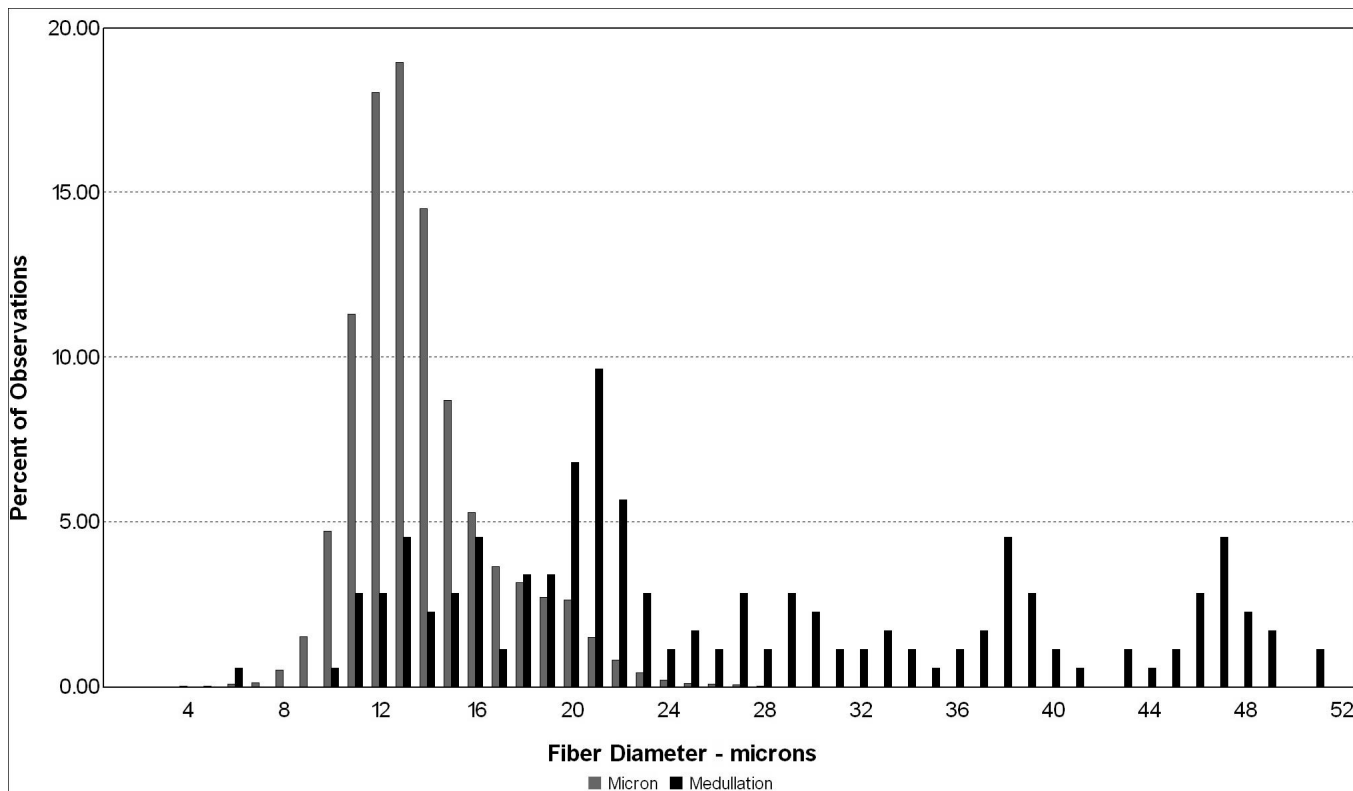

This Test Performed According to I.W.T.O Method 47