

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Man in the Moon Farm, LLC/Brenda Landes
16108 Johns Creek Rd
New Castle VA 24127-6758 USA

Date: 05/08/19

Test No: 974341


Animal and Sample Description

Animal Name: Iceman
Breed: Alpaca(Huacaya)
Sex: Male
Color: White

Animal ID: XXXXX
Sample Location: Side
Sample Date: 04/23/19
Age: 06/01/18

Laboratory Data

Mean Fiber Diameter:	16.8 microns	Fibers Greater Than 30 microns:	0.6 %
Standard Deviation:	3.3 microns	Comfort Factor:	99.4 %
Coefficient of Variation:	19.7 %	Mean Curvature:	43.2 deg/mm
Spin Fineness:	16.1 microns	SD Curvature:	21.2 deg/mm

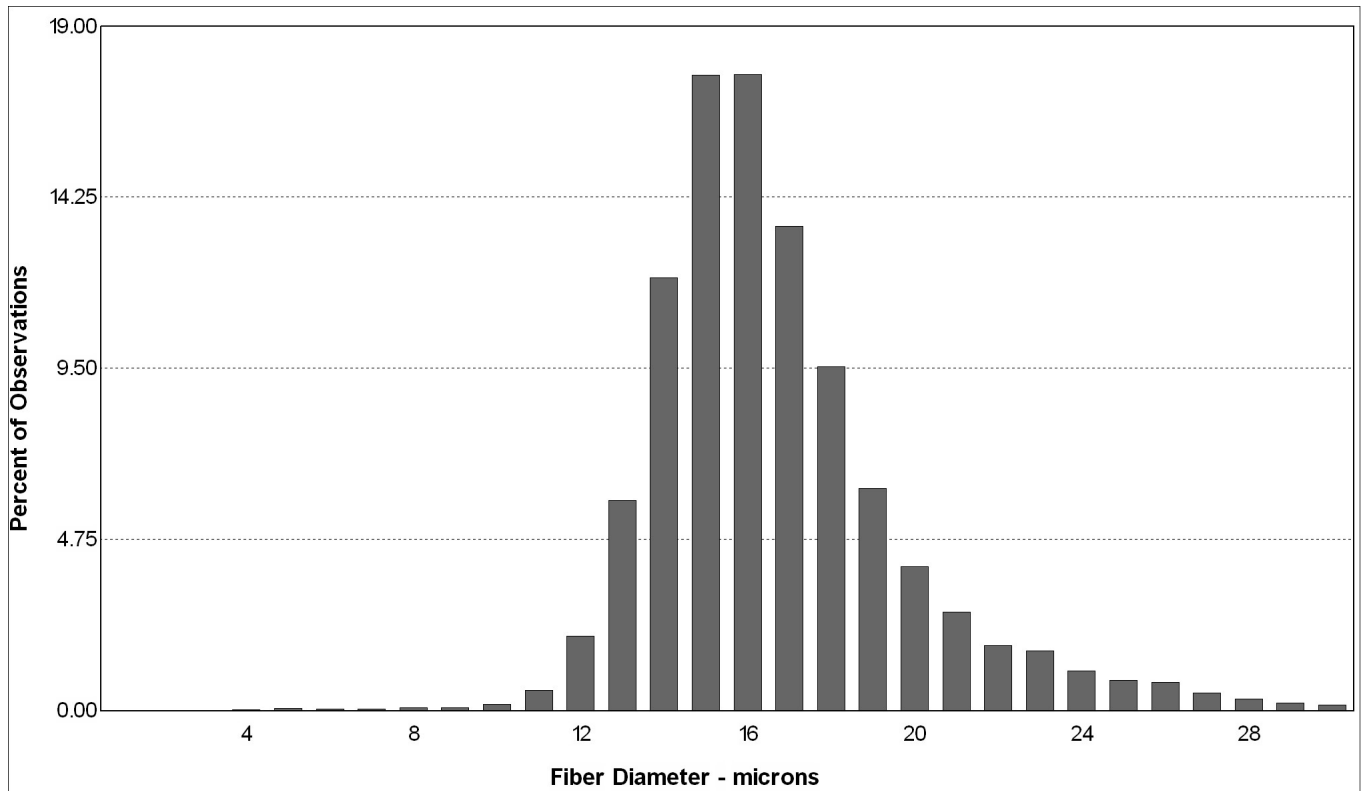

This Test Performed According to I.W.T.O Method 47