



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Alpaca Of Whitaker Mill/Elizabeth Hicks  
1212 Whitaker Mill Rd  
Joppa MD 21085 USA

09/08/17

Test No: 952100


### Animal and Sample Description

**Animal Name:** Hemlock Of Whitaker's Mill  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** True Black

**Animal ID:** 35188216  
**Sample Location:** Side  
**Sample Date:** 04/29/17  
**Age:** 10/12/15

### Laboratory Data

**Mean Fiber Diameter:** 25.4 microns  
**Standard Deviation:** 4.8 microns  
**Coefficient of Variation:** 18.9 %  
**Fibers Greater Than 30 microns:** 12.5 %

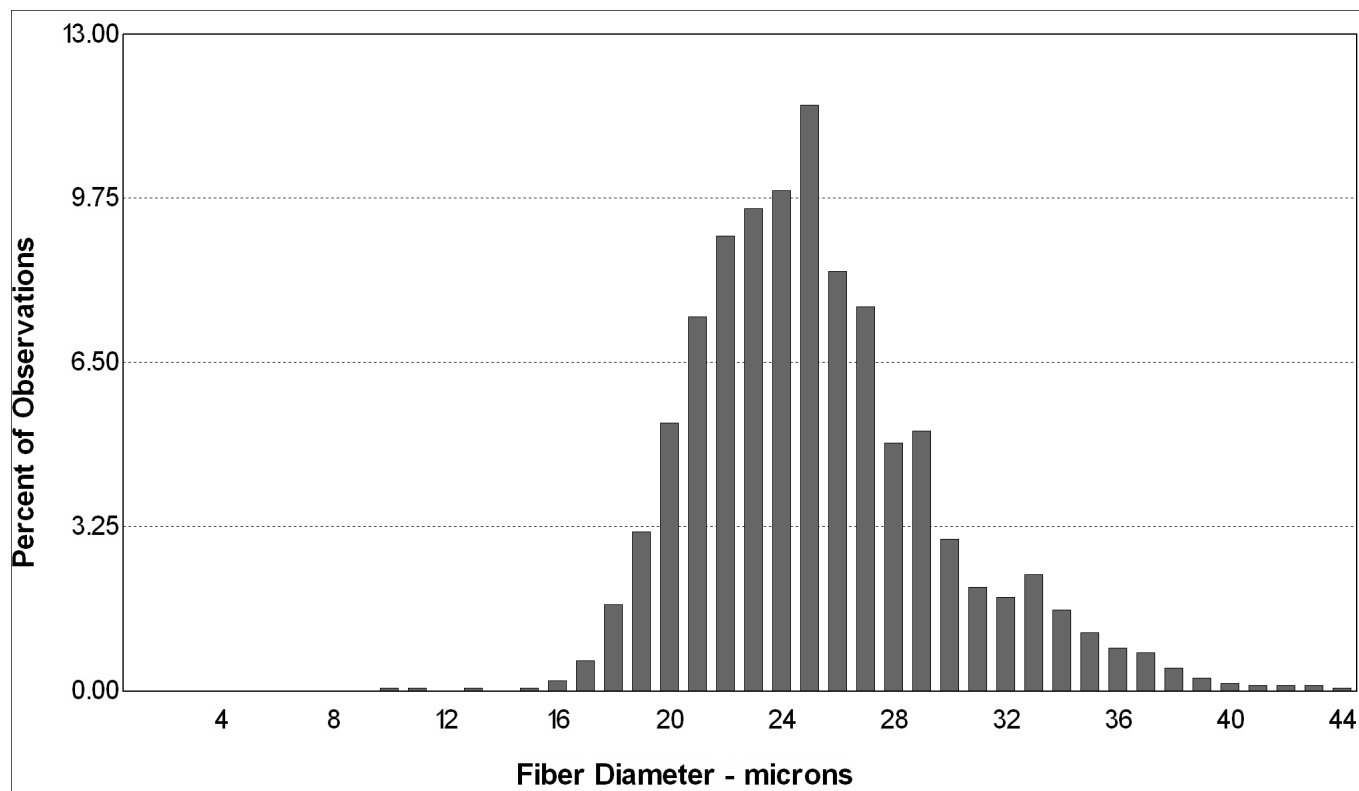

This Test Performed According to I.W.T.O Method 12