



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Willow Wind Farm/Annie Hunt
548 East State Highway 56
Berthoud CO 80513 USA

09/23/17

Test No: 952920


Animal and Sample Description

Animal Name: Springtoo Gigi
Breed: Alpaca(Huacaya)
Sex: Female
Color: True Black

Animal ID: 35025924
Sample Location: Side
Sample Date: 05/29/17
Age: 09/17/15

Laboratory Data

Mean Fiber Diameter:	18.8 microns	Spin Fineness:	18.1 microns
Standard Deviation:	3.7 microns	Mean Curvature (deg/mm):	40.1
Coefficient of Variation:	19.6 %	SD Curvature (deg/mm):	23.3
Fibers Greater Than 30 microns:	1.1 %	Comfort Factor:	98.9 %

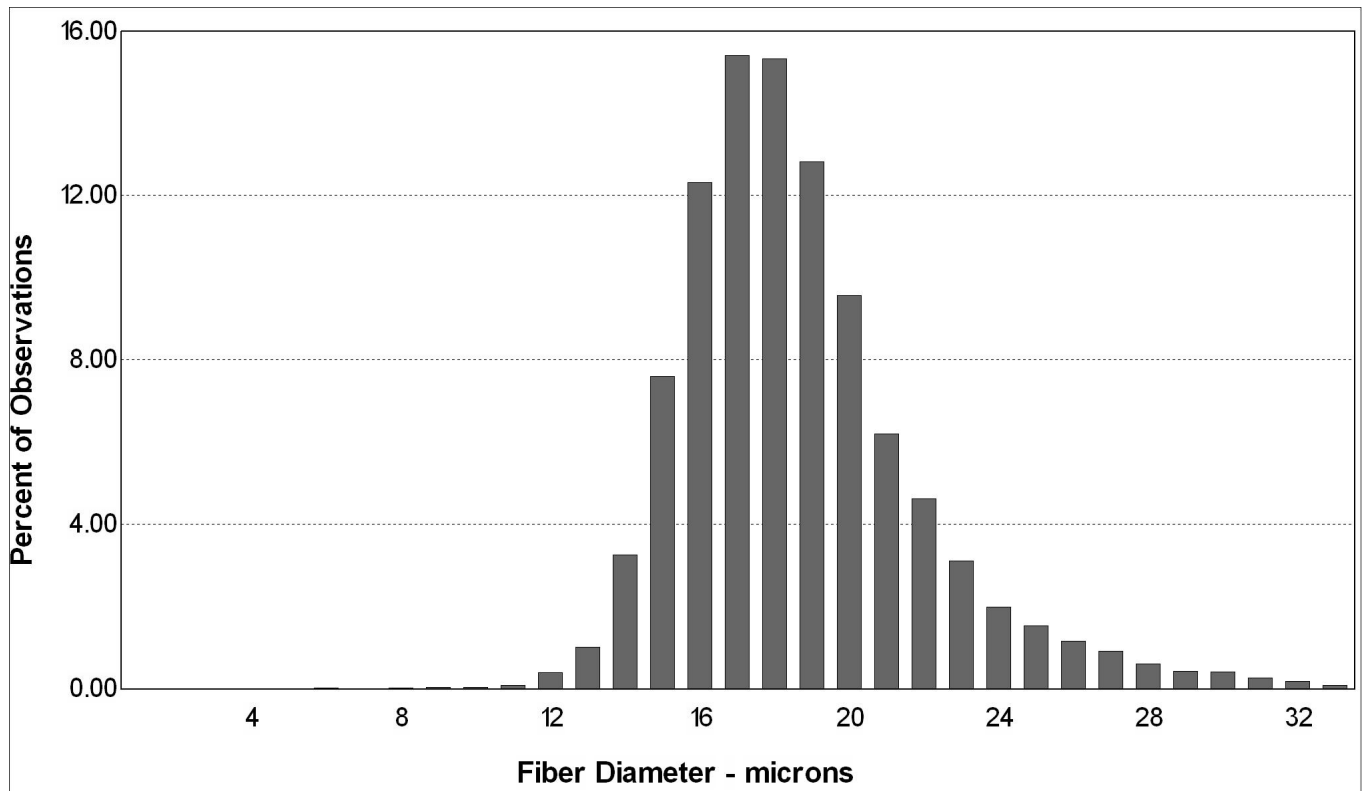

This Test Performed According to I.W.T.O Method 47