



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Willow Wind Farm/Annie Hunt
548 East State Highway 56
Berthoud CO 80513 USA

09/23/17

Test No: 952903


Animal and Sample Description

Animal Name: Springtoo Stella Artois
Breed: Alpaca(Huacaya)
Sex: Female
Color: Med Brown

Animal ID: 31862967
Sample Location: Side
Sample Date: 05/29/17
Age: 09/17/10

Laboratory Data

Mean Fiber Diameter:	20.6 microns	Spin Fineness:	20.2 microns
Standard Deviation:	4.5 microns	Mean Curvature (deg/mm):	42.8
Coefficient of Variation:	21.7 %	SD Curvature (deg/mm):	24.6
Fibers Greater Than 30 microns:	3.5 %	Comfort Factor:	96.5 %

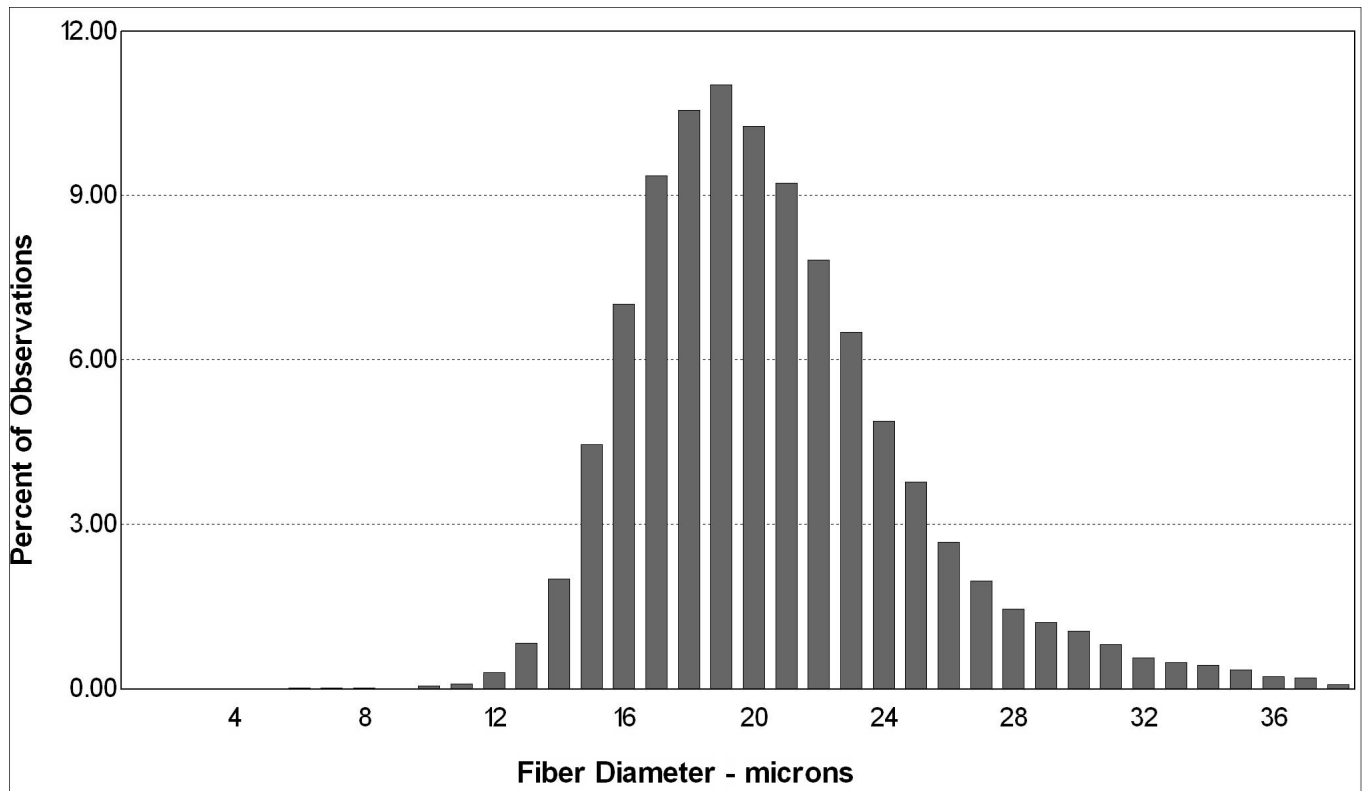

This Test Performed According to I.W.T.O Method 47