



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

CrimpHaven Alpacas, LLC/Jeanne Wilson
4165 West Midland Trail
Lexington VA 24450

04/26/16

Test No: 920304


Animal and Sample Description

Animal Name: Encore's Bravo of CrimpHaven
Breed: Alpaca(Huacaya)
Sex: Male
Color: White

Animal ID: 35275480
Sample Location: Side (R)
Sample Date: 04/05/16
Age: 05/19/15

Laboratory Data

Mean Fiber Diameter: 18.1 microns
Standard Deviation: 3.4 microns
Coefficient of Variation: 18.9 %
Fibers Greater Than 30 microns: 0.6 %

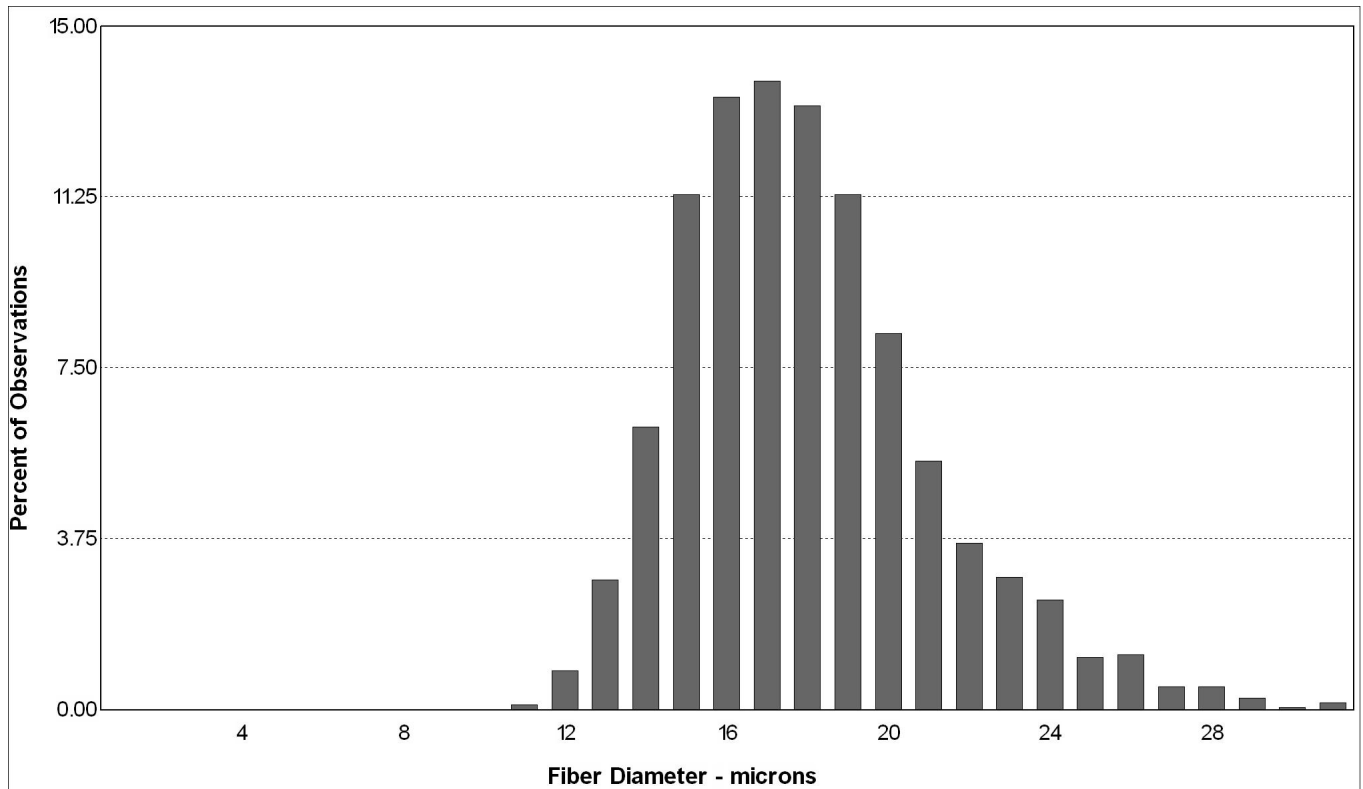

This Test Performed According to I.W.T.O Method 12