



Yocom-McColl Testing Laboratories, Inc.
540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

**Optical Fiber Diameter Analyser (OFDA100)
Micron Test Report**

Bay Shore Alpacas/Glen Kirby
2797 Smithfield Rd
St Stephens Church VA 23148 USA

09/24/15

Test No: 915275


Animal and Sample Description

Animal Name: Truman
Breed: Alpaca(Huacaya)
Sex: Male
Color: XXXXX

Animal ID: XXXXX
Sample Location: Side
Sample Date: 04/10/15
Age: 11/24/14

Laboratory Data

Mean Fiber Diameter:	16.6 microns	Spin Fineness:	16.7 microns
Standard Deviation:	4.1 microns	Mean Curvature (deg/mm):	40.5
Coefficient of Variation:	24.8 %	SD Curvature (deg/mm):	24.1
Fibers Greater Than 30 microns:	0.8 %	Comfort Factor:	99.2 %

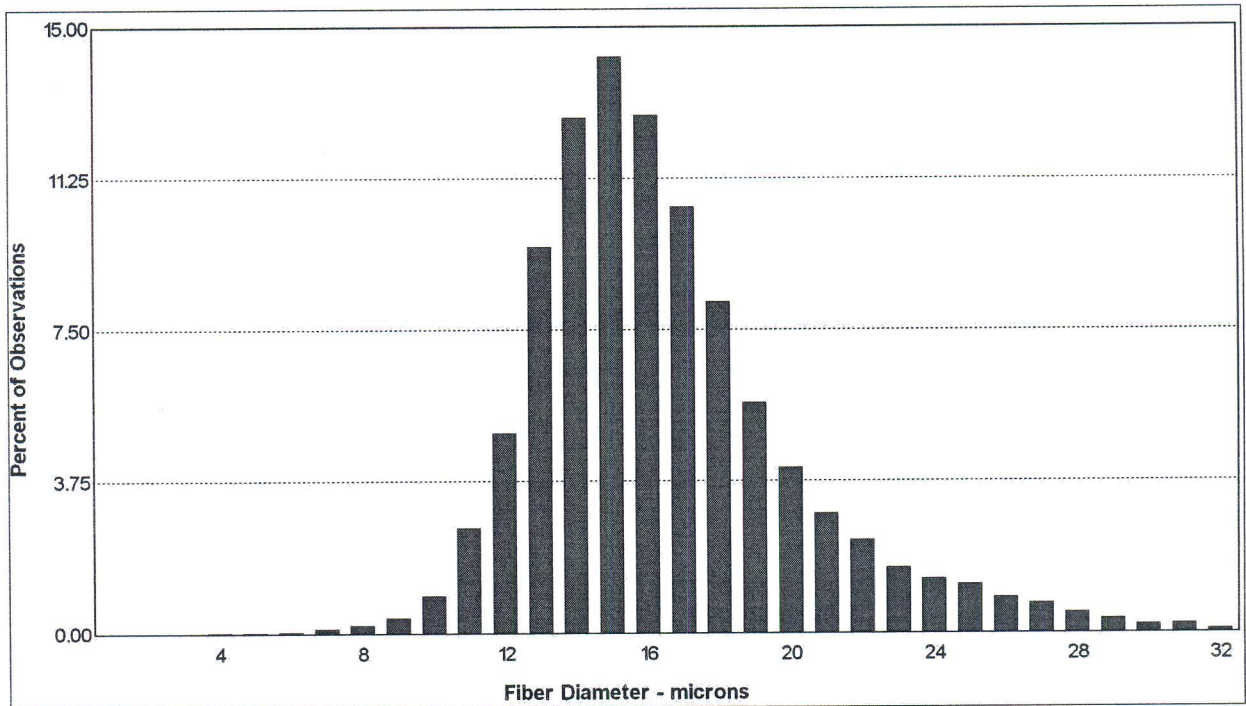

This Test Performed According to I.W.T.O Method 47