



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Grazing Hills Alpacas/Katie DeWinkle  
1042 Four Mile Rd  
Viola ID 83872 USA

08/18/16

Test No: 932913


### Animal and Sample Description

**Animal Name:** The Perazzi Mirage at Grazing Hills  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** Lt Brown

**Animal ID:** 32750850  
**Sample Location:** Side  
**Sample Date:** 06/09/16  
**Age:** 09/03/13

### Laboratory Data

**Mean Fiber Diameter:** 19.6 microns  
**Standard Deviation:** 4.4 microns  
**Coefficient of Variation:** 22.3 %  
**Fibers Greater Than 30 microns:** 2.1 %

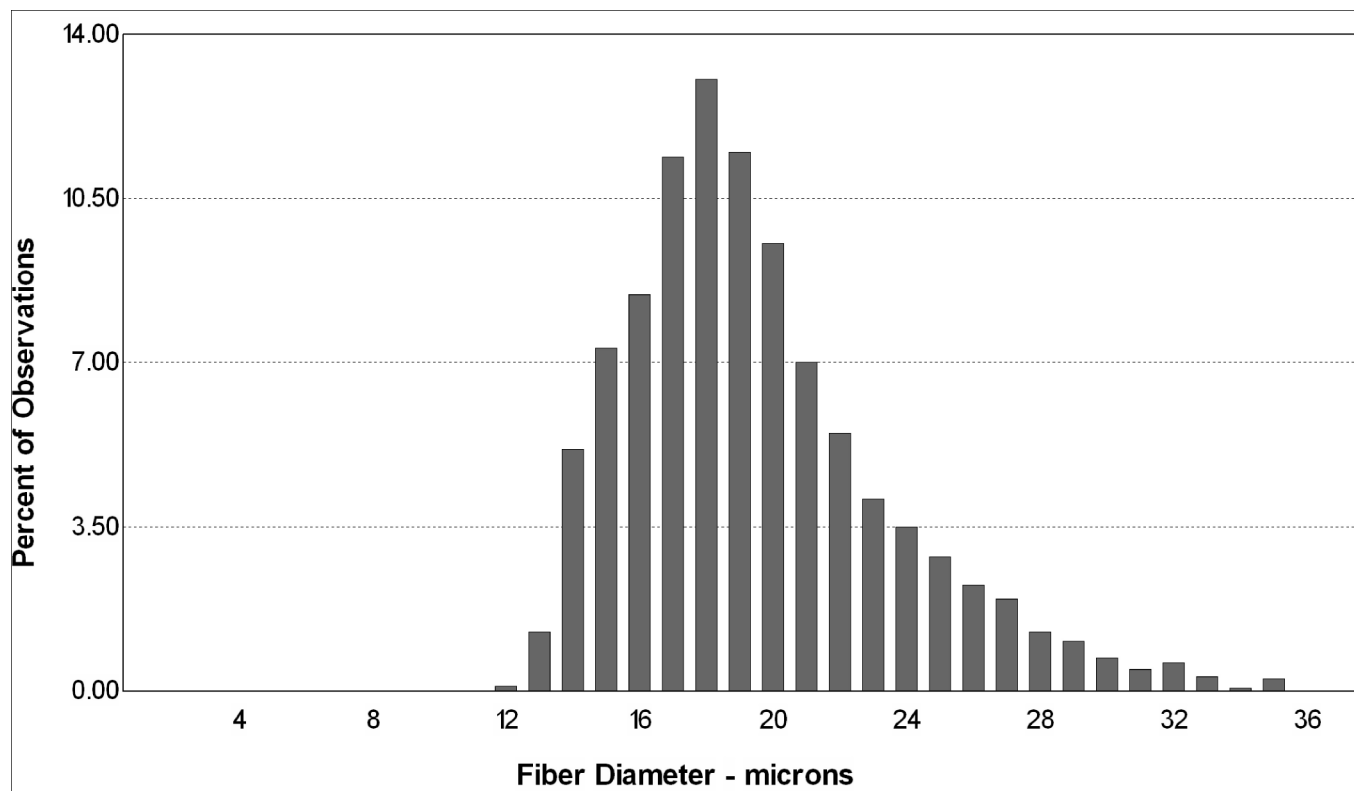

This Test Performed According to I.W.T.O Method 12