



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Nash Hill Alpacas/Rose Principato  
354 Tuckerton Rd  
Tabernacle NJ 08088 USA

01/08/18

Test No: 956072


### Animal and Sample Description

**Animal Name:** Cocoa of Willow Vale  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Dark Fawn

**Animal ID:** 35103226  
**Sample Location:** Blanket  
**Sample Date:** 05/15/17  
**Age:** 05/30/16

### Laboratory Data

**Mean Fiber Diameter:** 19.0 microns  
**Standard Deviation:** 4.2 microns  
**Coefficient of Variation:** 22.2 %  
**Fibers Greater Than 30 microns:** 1.6 %

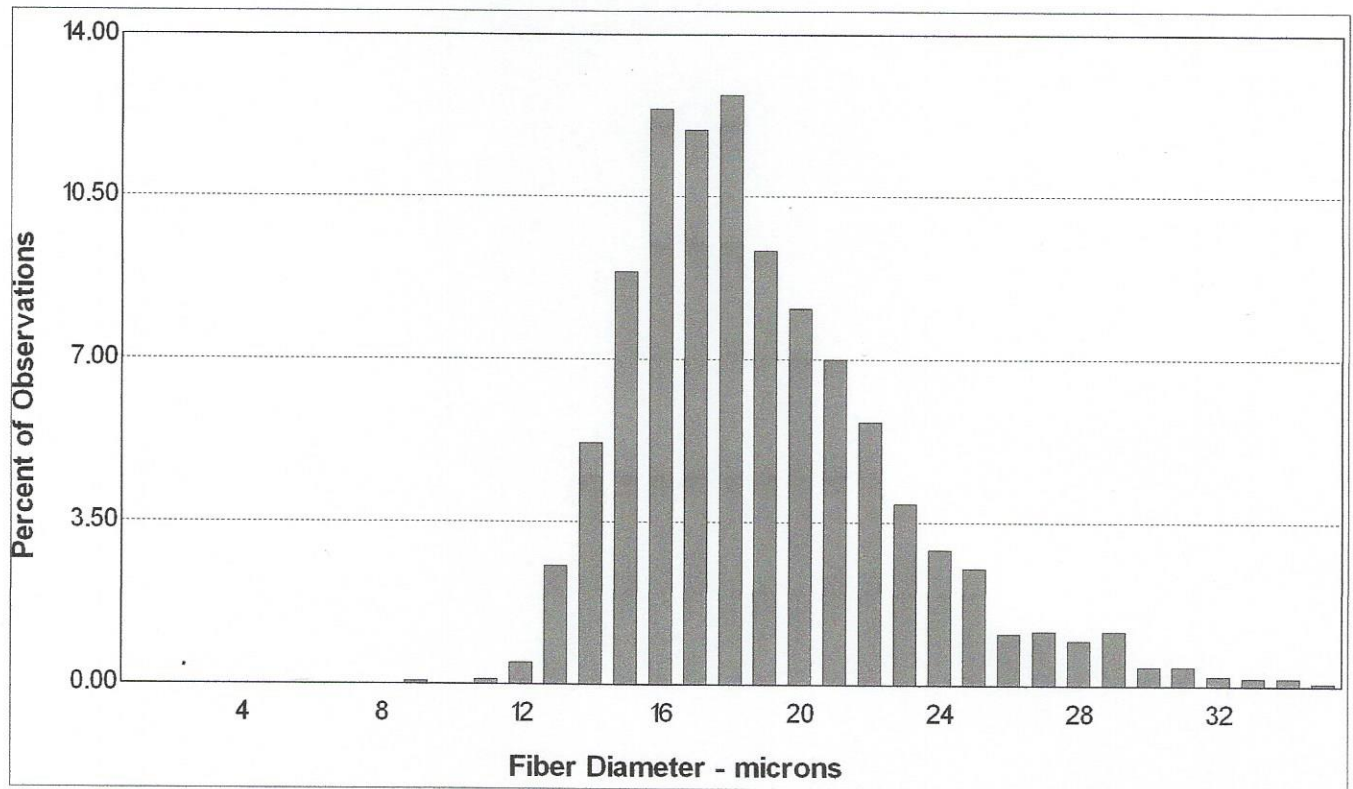

This Test Performed According to I.W.T.O Method 12