



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Nash Hill Alpacas/Rose Principato
354 Tuckerton Rd
Tabernacle NJ 08088 USA

01/08/18

Test No: 956083


Animal and Sample Description

Animal Name: Colton of Willow Vale
Breed: Alpaca(Huacaya)
Sex: Male
Color: Med Fawn

Animal ID: 35103219
Sample Location: Blanket
Sample Date: 05/15/17
Age: 09/06/16

Laboratory Data

Mean Fiber Diameter: 17.5 microns
Standard Deviation: 3.5 microns
Coefficient of Variation: 20.3 %
Fibers Greater Than 30 microns: 1.1 %

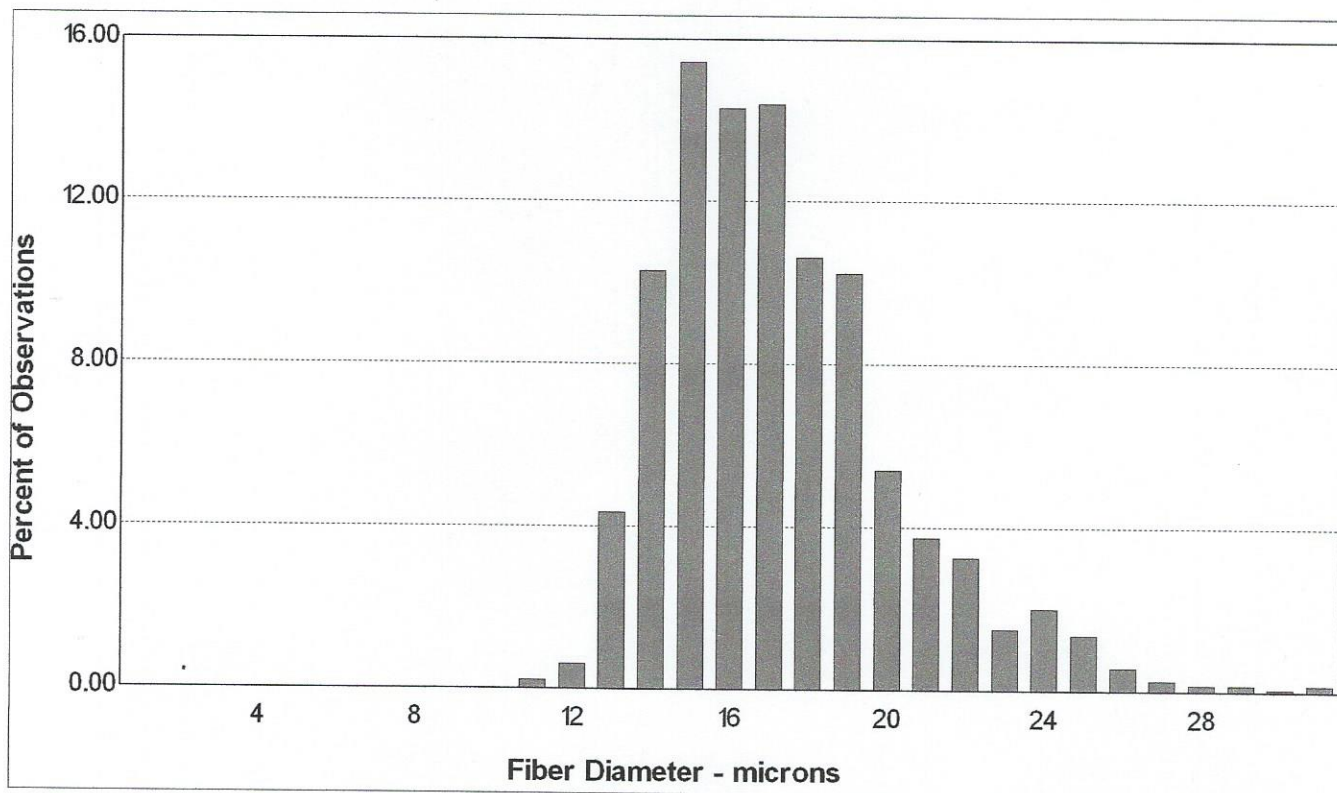

This Test Performed According to I.W.T.O Method 12