



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Nash Hill Alpacas/Rose Principato  
354 Tuckerton Rd  
Tabernacle NJ 08088 USA

01/08/18

Test No: 956077


### Animal and Sample Description

**Animal Name:** NHA Tucker  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** Lt Fawn

**Animal ID:** 32313857  
**Sample Location:** Blanket  
**Sample Date:** 05/15/17  
**Age:** 10/03/14

### Laboratory Data

**Mean Fiber Diameter:** 17.3 microns  
**Standard Deviation:** 3.4 microns  
**Coefficient of Variation:** 19.7 %  
**Fibers Greater Than 30 microns:** 0.5 %

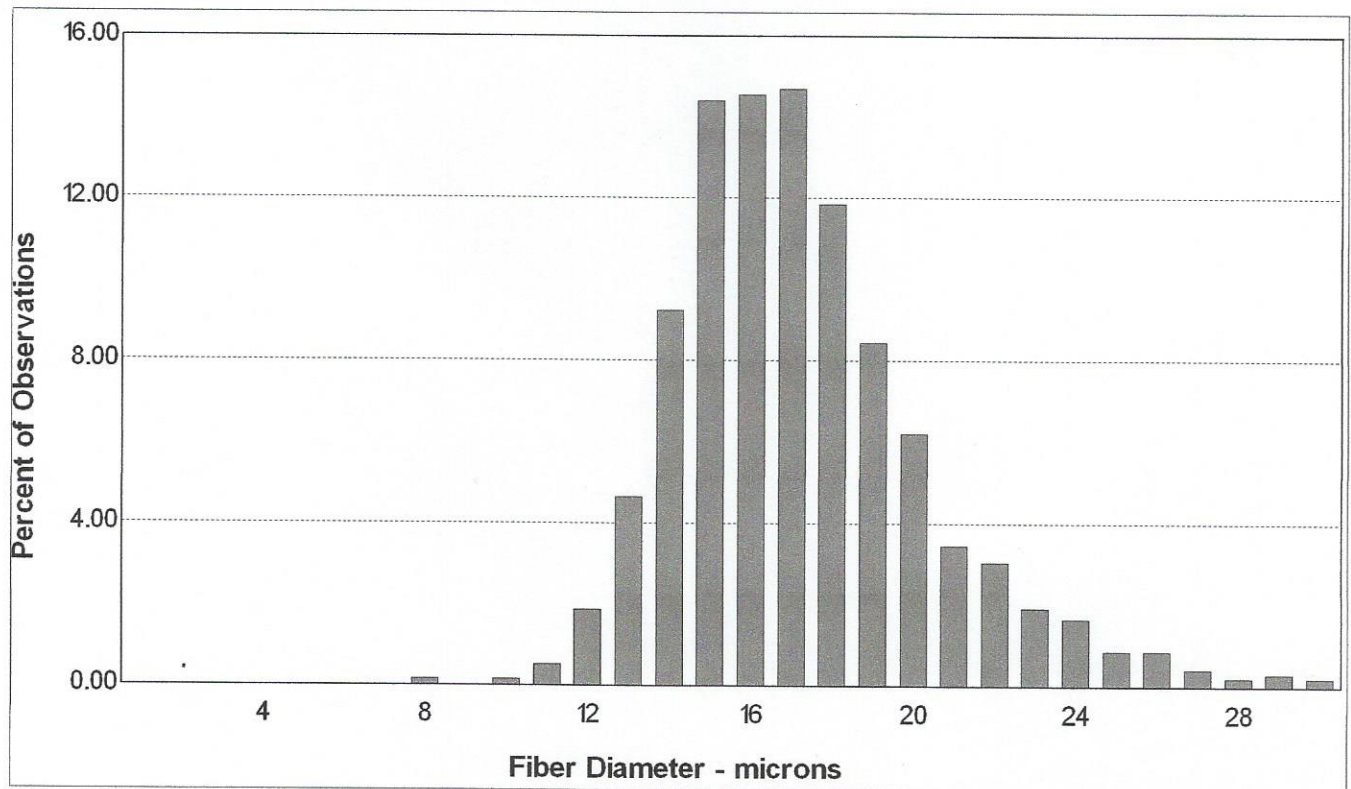

This Test Performed According to I.W.T.O Method 12