



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Sky Ridge Alpacas/Stacie Chavez
58150 Highway 197
Tygh Valley OR 97063

Date: 06/29/16

Test No: 925229


Animal and Sample Description

Animal Name: Sky Ridge Alpacas Stella
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: 32418286
Sample Location: Side
Sample Date: 05/24/16
Age: 08/20/15

Laboratory Data

Mean Fiber Diameter:	18.0 microns	Fibers Greater Than 30 microns:	0.5 %
Standard Deviation:	3.9 microns	Comfort Factor:	99.5 %
Coefficient of Variation:	21.8 %	Mean Curvature:	40.1 deg/mm
Spin Fineness:	17.6 microns	SD Curvature:	25.3 deg/mm

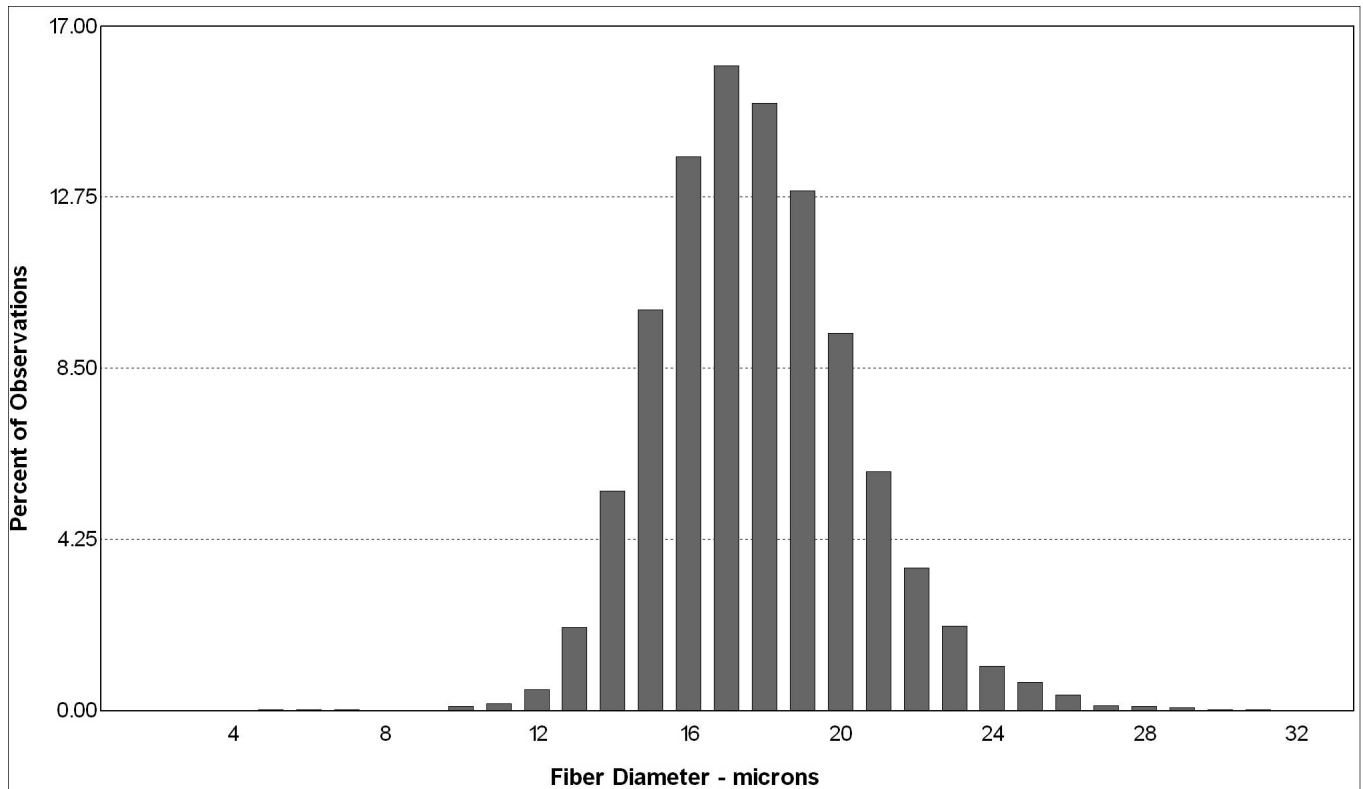

This Test Performed According to I.W.T.O Method 47