



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Sky Ridge Alpacas/Stacie Chavez
58150 Highway 197
Tygh Valley OR 97063

Date: 06/29/16

Test No: 925232


Animal and Sample Description

Animal Name: Sky Ridge Alpacas Jaguar
Breed: Alpaca(Huacaya)
Sex: Male
Color: Bay Black

Animal ID: 35012734
Sample Location: Side
Sample Date: 05/24/16
Age: 10/10/15

Laboratory Data

Mean Fiber Diameter:	20.5 microns	Fibers Greater Than 30 microns:	1.9 %
Standard Deviation:	4.0 microns	Comfort Factor:	98.1 %
Coefficient of Variation:	19.6 %	Mean Curvature:	36.0 deg/mm
Spin Fineness:	19.7 microns	SD Curvature:	22.8 deg/mm

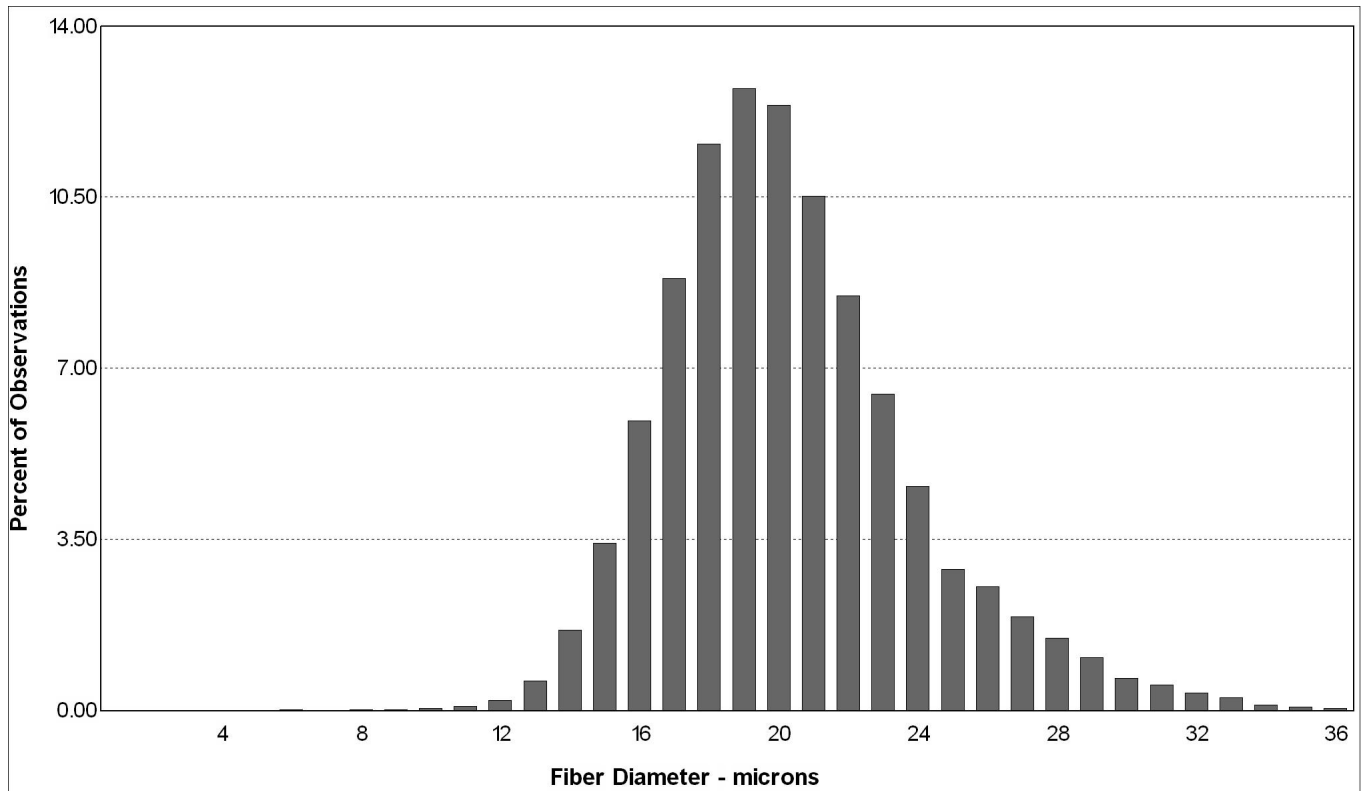

This Test Performed According to I.W.T.O Method 47