



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Sky Ridge Alpacas/Stacie Chavez
58150 Highway 197
Tygh Valley OR 97063

Date: 06/29/16

Test No: 925233


Animal and Sample Description

Animal Name: Sky Ridge Alpacas Max
Breed: Alpaca(Huacaya)
Sex: Male
Color: White

Animal ID: 32488920
Sample Location: Side
Sample Date: 05/24/16
Age: 08/10/15

Laboratory Data

Mean Fiber Diameter:	19.7 microns	Fibers Greater Than 30 microns:	1.3 %
Standard Deviation:	4.0 microns	Comfort Factor:	98.7 %
Coefficient of Variation:	20.4 %	Mean Curvature:	39.2 deg/mm
Spin Fineness:	19.1 microns	SD Curvature:	23.3 deg/mm

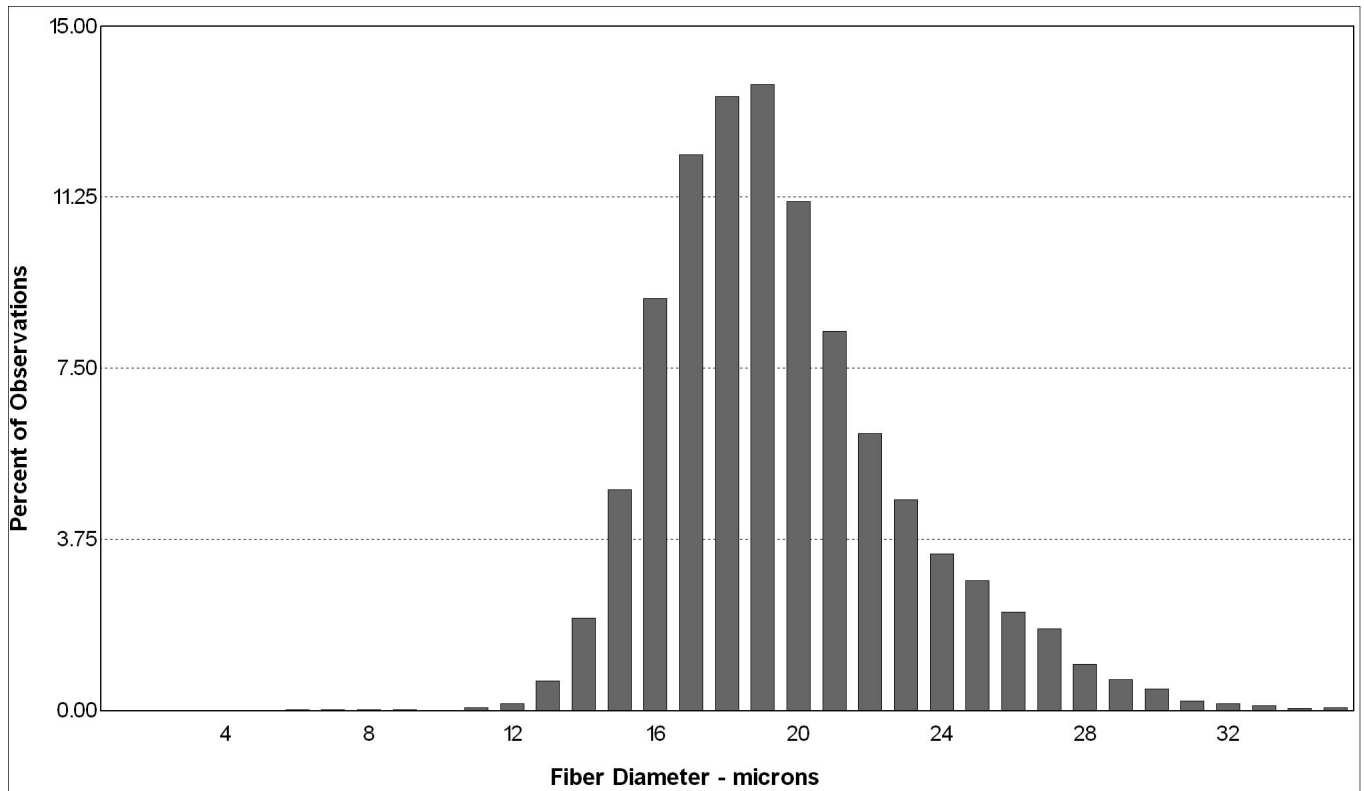

This Test Performed According to I.W.T.O Method 47