



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Sky Ridge Alpacas/Stacie Chavez
58150 Highway 197
Tygh Valley OR 97063

06/13/18

Test No: 961658


Animal and Sample Description

Animal Name: Dancer
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: 35421740
Sample Location: Hip (L)
Sample Date: 05/04/18
Age: 10/04/17

Laboratory Data

Mean Fiber Diameter:	15.4 microns	Spin Fineness:	15.1 microns
Standard Deviation:	3.3 microns	Mean Curvature (deg/mm):	39.1
Coefficient of Variation:	21.4 %	SD Curvature (deg/mm):	23.1
Fibers Greater Than 30 microns:	0.4 %	Comfort Factor:	99.6 %

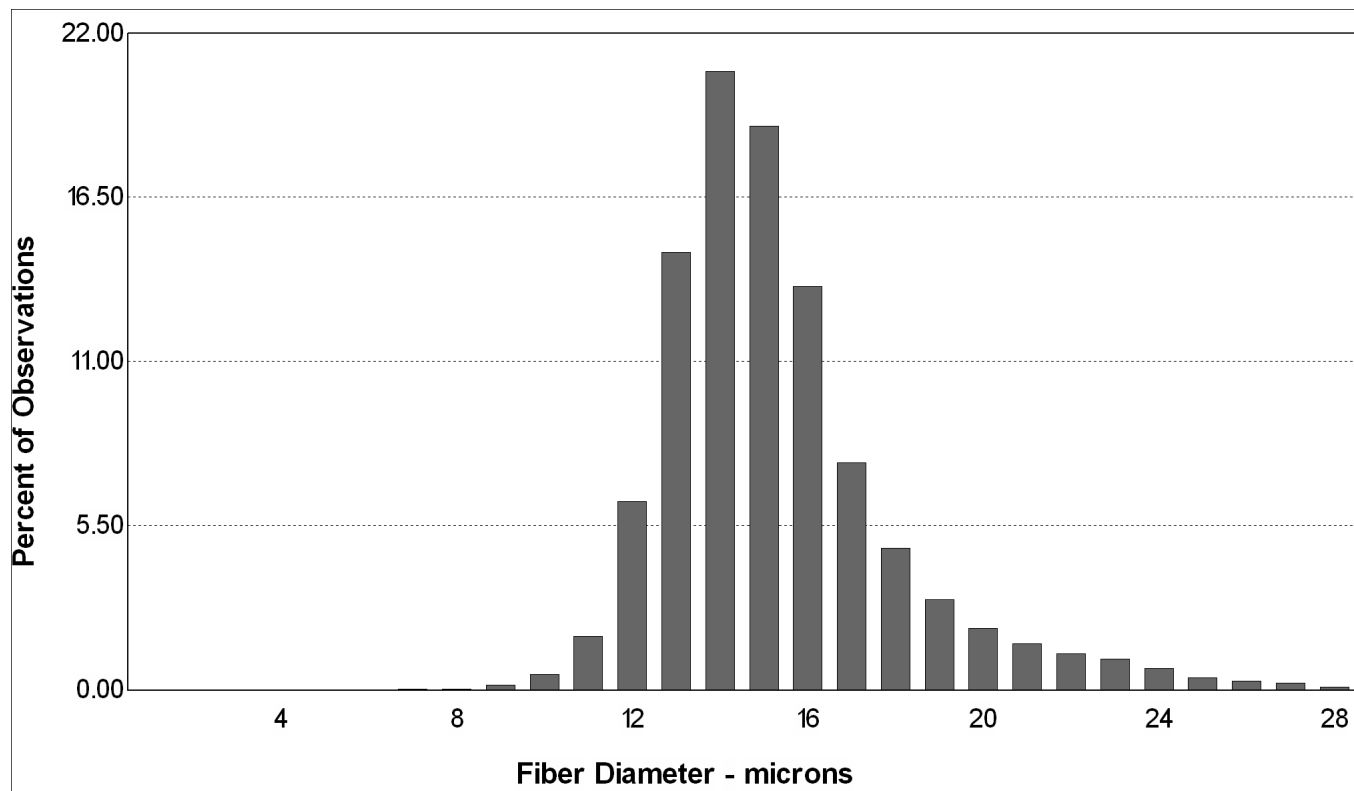

This Test Performed According to I.W.T.O Method 47