

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

South Mountain Alpacas/Stacie Chavez
5 Sage Lane
Edgewood NM 87015 USA

07/27/13

Test No: 463395


Animal and Sample Description

Animal Name: Snowmass Accoyo Distinction
Breed: Alpaca(Huacaya)
Sex: Male
Color: White

Animal ID: 32310658
Sample Location: Side
Sample Date: 05/22/13
Age: 11/16/11

Laboratory Data

| | | | |
|---------------------------------|--------------|--------------------------|--------------|
| Mean Fiber Diameter: | 17.5 microns | Spin Fineness: | 16.8 microns |
| Standard Deviation: | 3.4 microns | Mean Curvature (deg/mm): | 50.3 |
| Coefficient of Variation: | 19.5 % | SD Curvature (deg/mm): | 26.3 |
| Fibers Greater Than 30 microns: | 0.4 % | Comfort Factor: | 99.6 % |

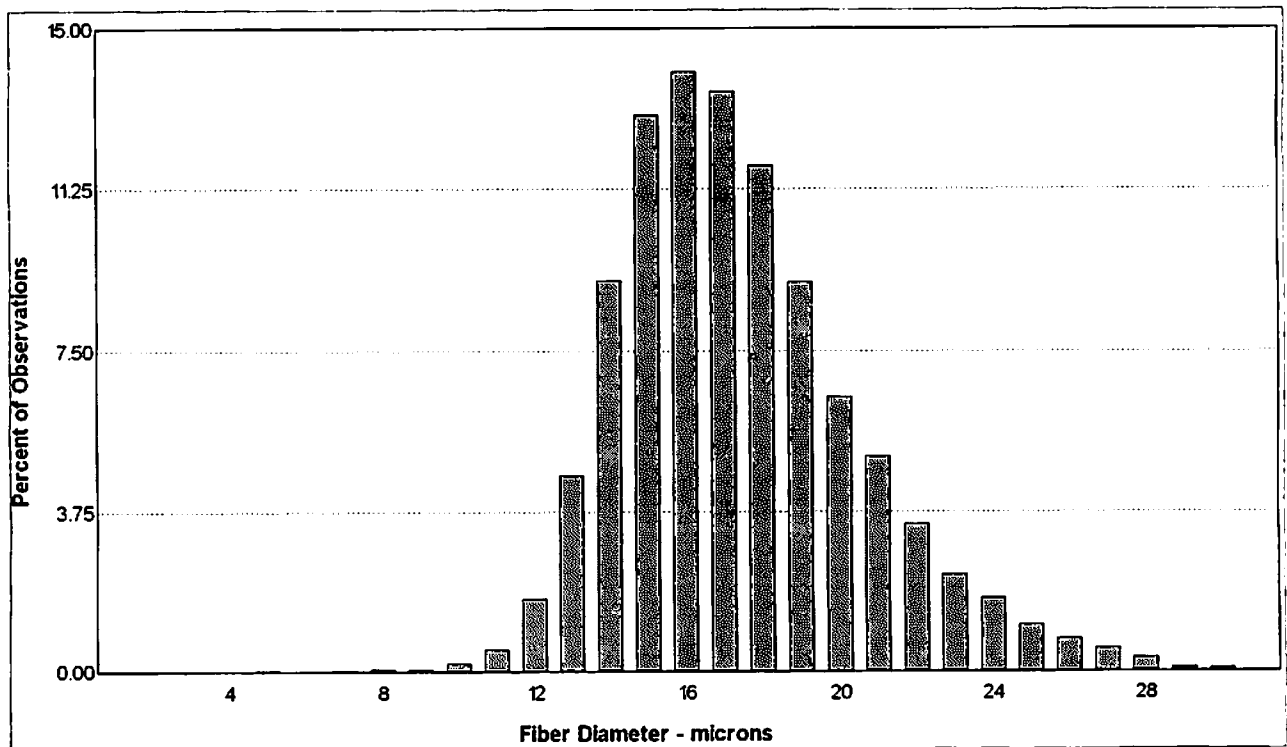

This Test Performed According to I.W.T.O Method 47