



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Cherry Blossom Alpacas LLC/Brooke White
2877 Godding Hollow Pkwy
Longmont CO 80504 USA

07/12/17

Test No: 945697


Animal and Sample Description

Animal Name: Daybreak's Darla
Breed: Alpaca(Huacaya)
Sex: Female
Color: Lt Fawn

Animal ID: 32072525
Sample Location: Mid Side
Sample Date: 05/27/17
Age: 09/28/11

Laboratory Data

Mean Fiber Diameter: 24.6 microns
Standard Deviation: 4.5 microns
Coefficient of Variation: 18.2 %
Fibers Greater Than 30 microns: 8.6 %

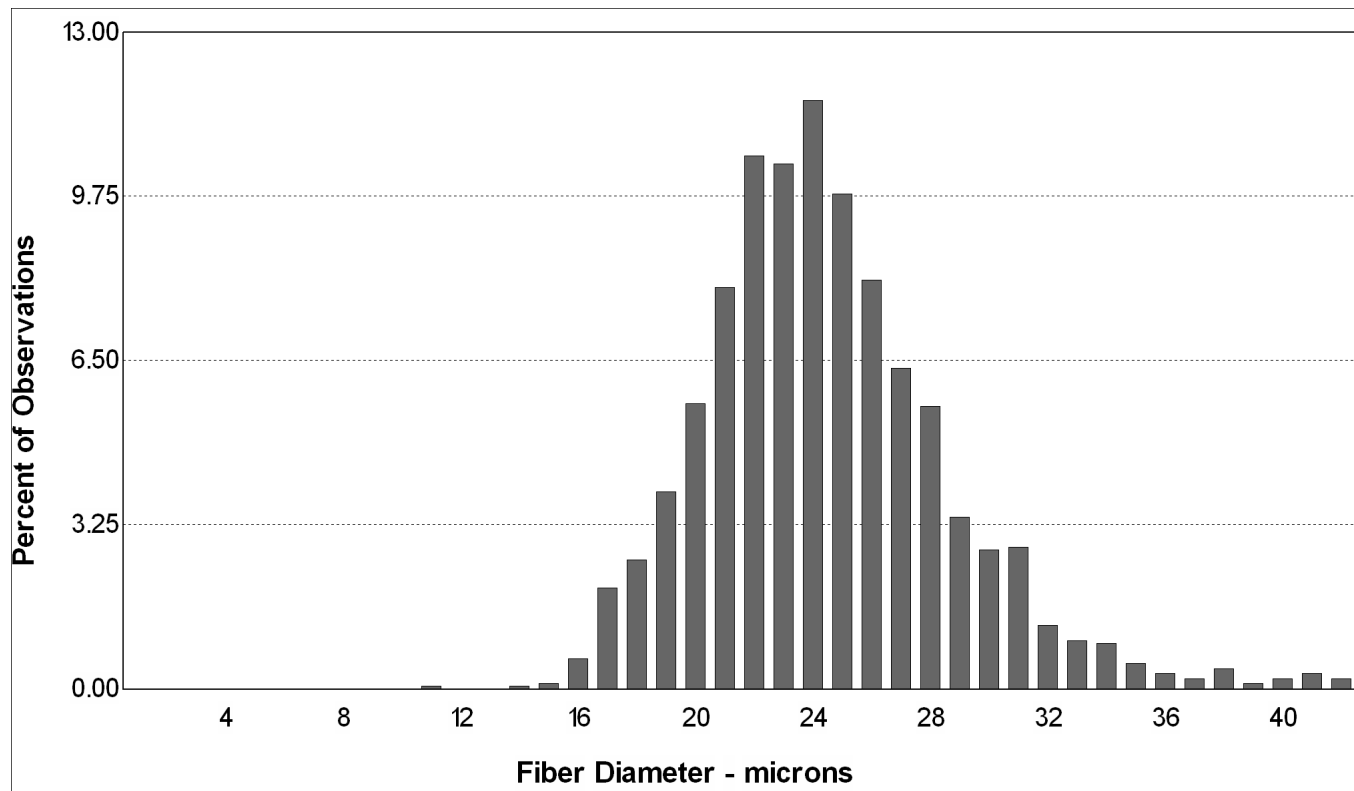

This Test Performed According to I.W.T.O Method 12