



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Sirolan Laserscan Micron Test Report

Wilkins Livestock Ranch/Mike & Janet Wilkins  
1405 Rd 12  
Geneva NE 68361 USA

08/30/19

Test No: 971365


### Animal and Sample Description

**Animal Name:** WLK Ryker  
**Breed:** Alpaca(Suri)  
**Sex:** Male  
**Color:** Lt Fawn

**Animal ID:** 35426783  
**Sample Location:** Mid Side  
**Sample Date:** 11/12/18  
**Age:** 10/11/17

### Laboratory Data

**Mean Fiber Diameter:** 19.5 microns  
**Standard Deviation:** 3.9 microns  
**Coefficient of Variation:** 19.9 %  
**Fibers Greater Than 30 microns:** 1.3 %

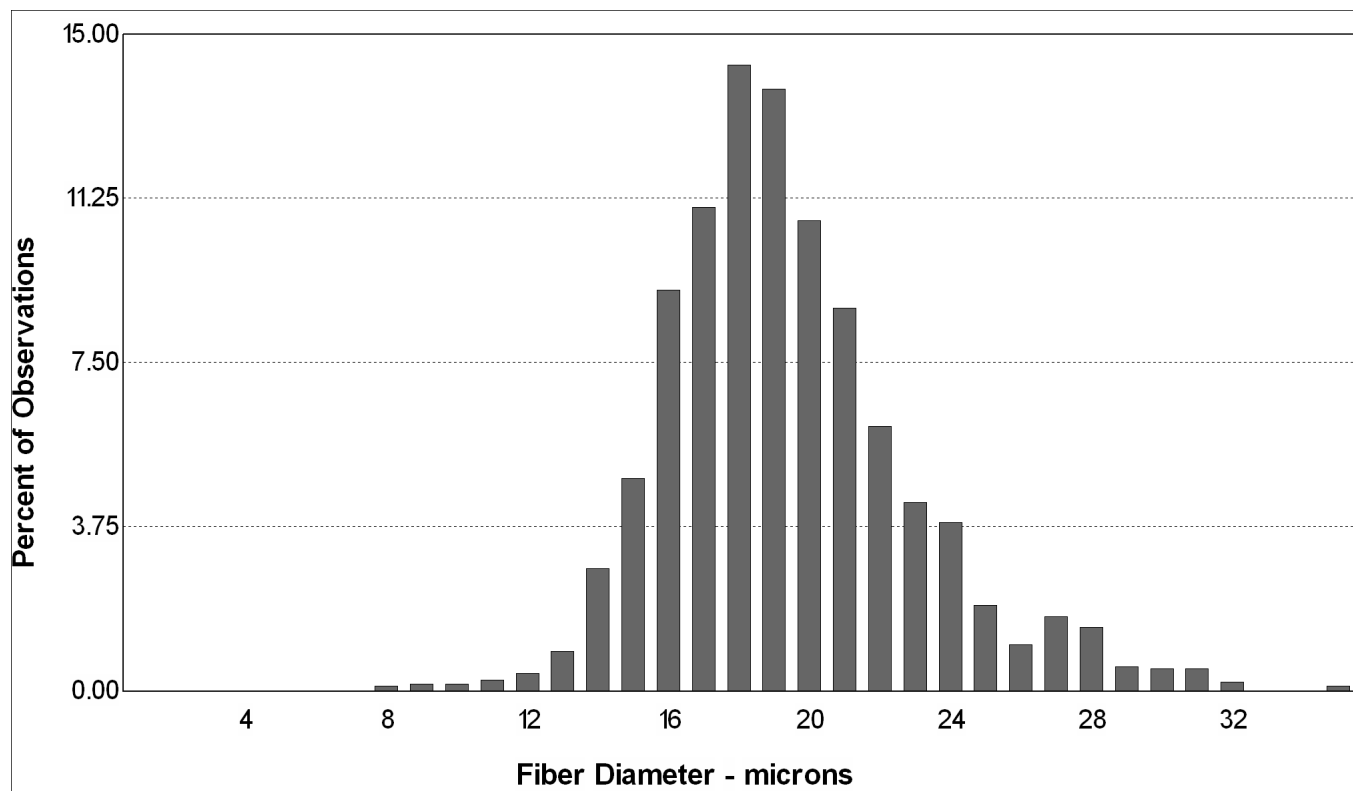

This Test Performed According to I.W.T.O Method 12