



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Cherlyn Hills Alpaca Farm/Cheryl Neal  
2345 Cortland Virgil Road  
Cortland NY 13045 USA

10/18/19

Test No: 978424


### Animal and Sample Description

**Animal Name:** Sun Shadow  
**Breed:** Alpaca(Huacaya)  
**Sex:** Male  
**Color:** Black

**Animal ID:** 35092841  
**Sample Location:** Side  
**Sample Date:** 06/07/19  
**Age:** 06/16/18

### Laboratory Data

<b>Mean Fiber Diameter:</b>	22.6 microns	<b>Spin Fineness:</b>	22.6 microns
<b>Standard Deviation:</b>	5.5 microns	<b>Mean Curvature (deg/mm):</b>	24.6
<b>Coefficient of Variation:</b>	24.4 %	<b>SD Curvature (deg/mm):</b>	17.7
<b>Fibers Greater Than 30 microns:</b>	8.0 %	<b>Comfort Factor:</b>	92.0 %

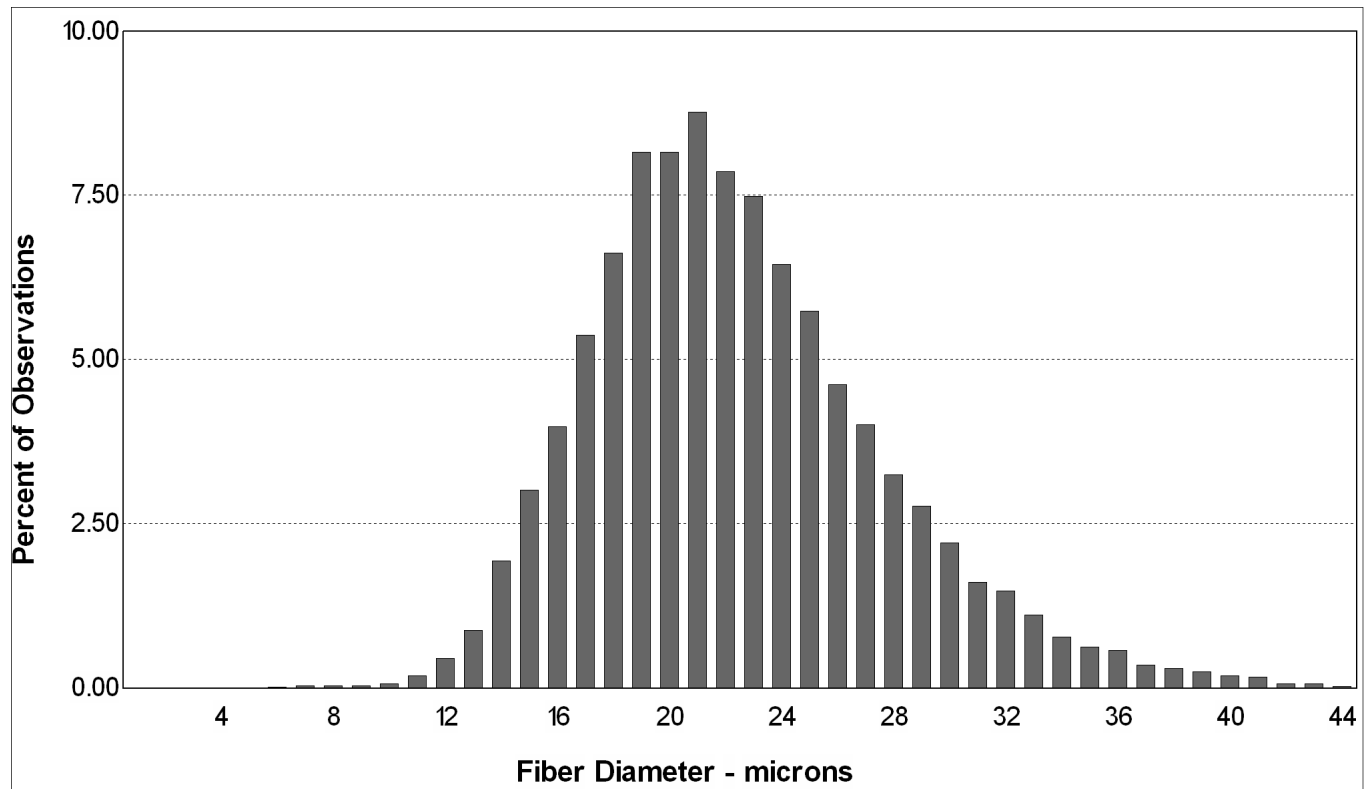

This Test Performed According to I.W.T.O Method 47