



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Sweet Valley Suris/Kristie Smoker
5701 Valley Glen Rd
Annville PA 17003-9158 USA

Date: 09/04/19

Test No: 983027


Animal and Sample Description

Animal Name: Patience
Breed: Alpaca(Suri)
Sex: Female
Color: XXXXX

Animal ID: 35440529
Sample Location: Side
Sample Date: 05/21/18
Age: 08/05/16

Laboratory Data

Mean Fiber Diameter:	24.4 microns	Fibers Greater Than 30 microns:	14.0 %
Standard Deviation:	6.9 microns	Comfort Factor:	86.0 %
Coefficient of Variation:	28.4 %	Mean Curvature:	9.7 deg/mm
Spin Fineness:	25.5 microns	SD Curvature:	13.0 deg/mm

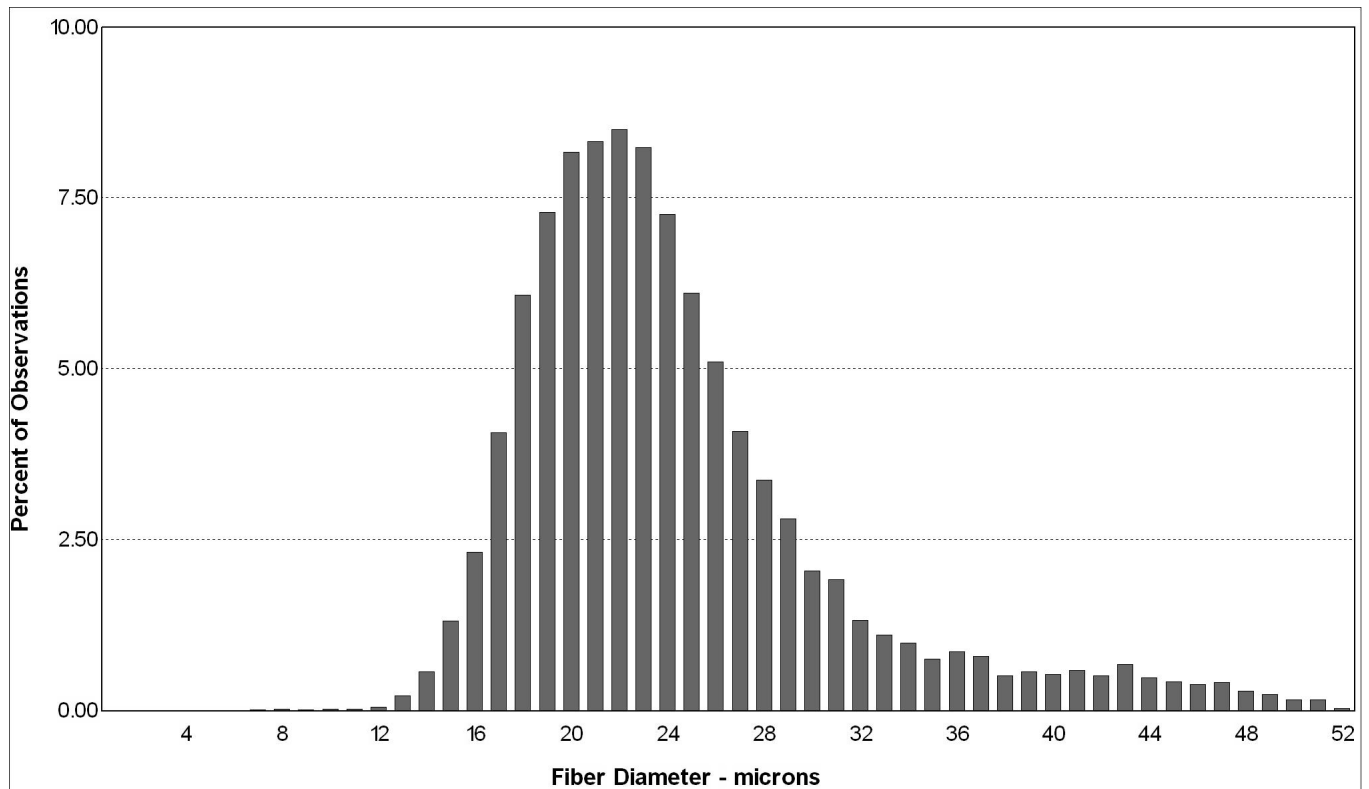

This Test Performed According to I.W.T.O Method 47