



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Sweet Valley Suris/Kristie Smoker
5701 Valley Glen Rd
Annville PA 17003-9158 USA

Date: 09/04/19

Test No: 983030


Animal and Sample Description

Animal Name: SVS Hannah
Breed: Alpaca(Suri)
Sex: Female
Color: XXXXX

Animal ID: 32370591
Sample Location: Side
Sample Date: 05/21/18
Age: 09/01/12

Laboratory Data

Mean Fiber Diameter:	26.1 microns	Fibers Greater Than 30 microns:	16.2 %
Standard Deviation:	5.3 microns	Comfort Factor:	83.8 %
Coefficient of Variation:	20.5 %	Mean Curvature:	8.3 deg/mm
Spin Fineness:	25.3 microns	SD Curvature:	9.5 deg/mm

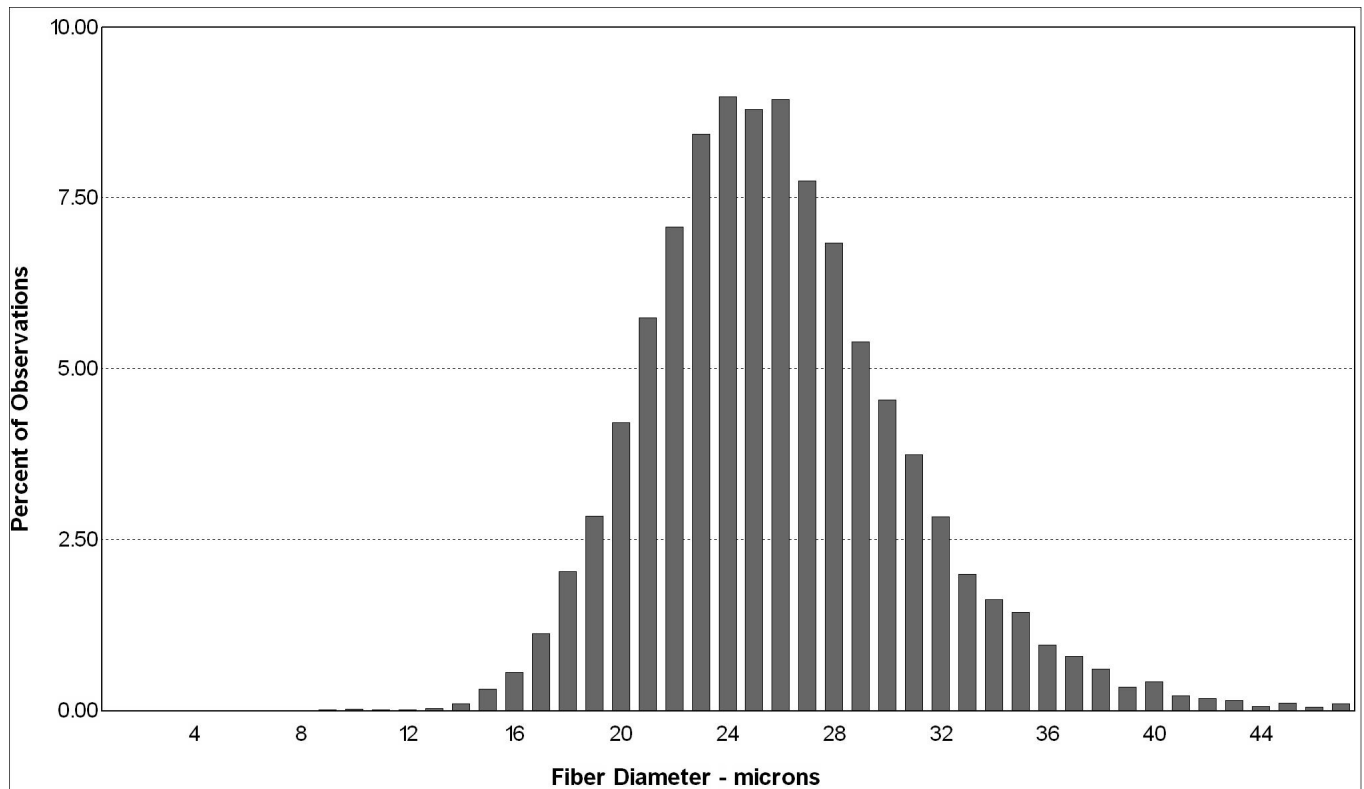

This Test Performed According to I.W.T.O Method 47