



# Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

## Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Fun In The Country Alpacas/Kimberly Les  
10337 Washburn Road  
Columbiaville MI 48421 USA

02/25/20

Test No: 987328


### Animal and Sample Description

**Animal Name:** Belle of the Ball  
**Breed:** Alpaca(Huacaya)  
**Sex:** Female  
**Color:** Beige

**Animal ID:** 32376180  
**Sample Location:** Side  
**Sample Date:** 04/20/19  
**Age:** 06/14/11

### Laboratory Data

|  |              |                                 |              |
|--|--------------|---------------------------------|--------------|
| <b>Mean Fiber Diameter:</b>            | 19.1 microns | <b>Spin Fineness:</b>           | 18.0 microns |
| <b>Standard Deviation:</b>             | 3.3 microns  | <b>Medullated Fibers:</b>       | 0.0 %        |
| <b>Coefficient of Variation:</b>       | 17.4 %       | <b>Mean Curvature (deg/mm):</b> | 49.5         |
| <b>Fibers Greater Than 30 microns:</b> | 0.6 %        | <b>SD Curvature (deg/mm):</b>   | 28.6         |

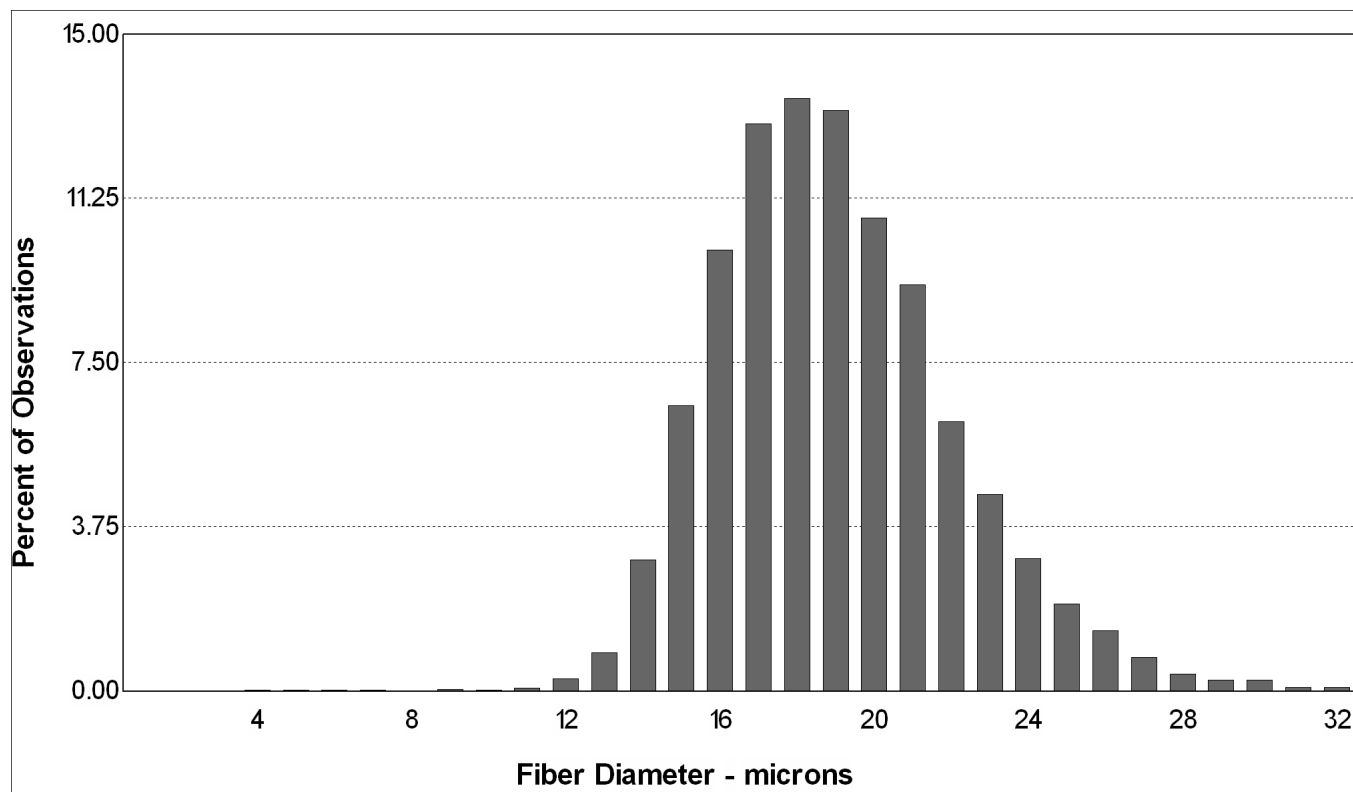

This Test Performed According to I.W.T.O Method 47