



Yocom-McColl Testing Laboratories, Inc.
540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

**Sirolan Laserscan
Micron Test Report**

Squire Creek Ranch/Michael DeDear
41017 Squire Creek Rd
Arlington WA 98223 USA

09/14/10

Test No: 390738


Animal and Sample Description

Animal Name: Premier's Gold Standard
Breed: Alpaca(Huacaya)
Sex: Male
Color: Medium Fawn

Animal ID: 30463189
Sample Location: Side
Sample Date: 05/15/10
Age: 06/15/09

Laboratory Data

Mean Fiber Diameter: 20.8 microns
Standard Deviation: 3.6 microns
Coefficient of Variation: 17.1 %
Fibers Greater Than 30 microns: 1.1 %

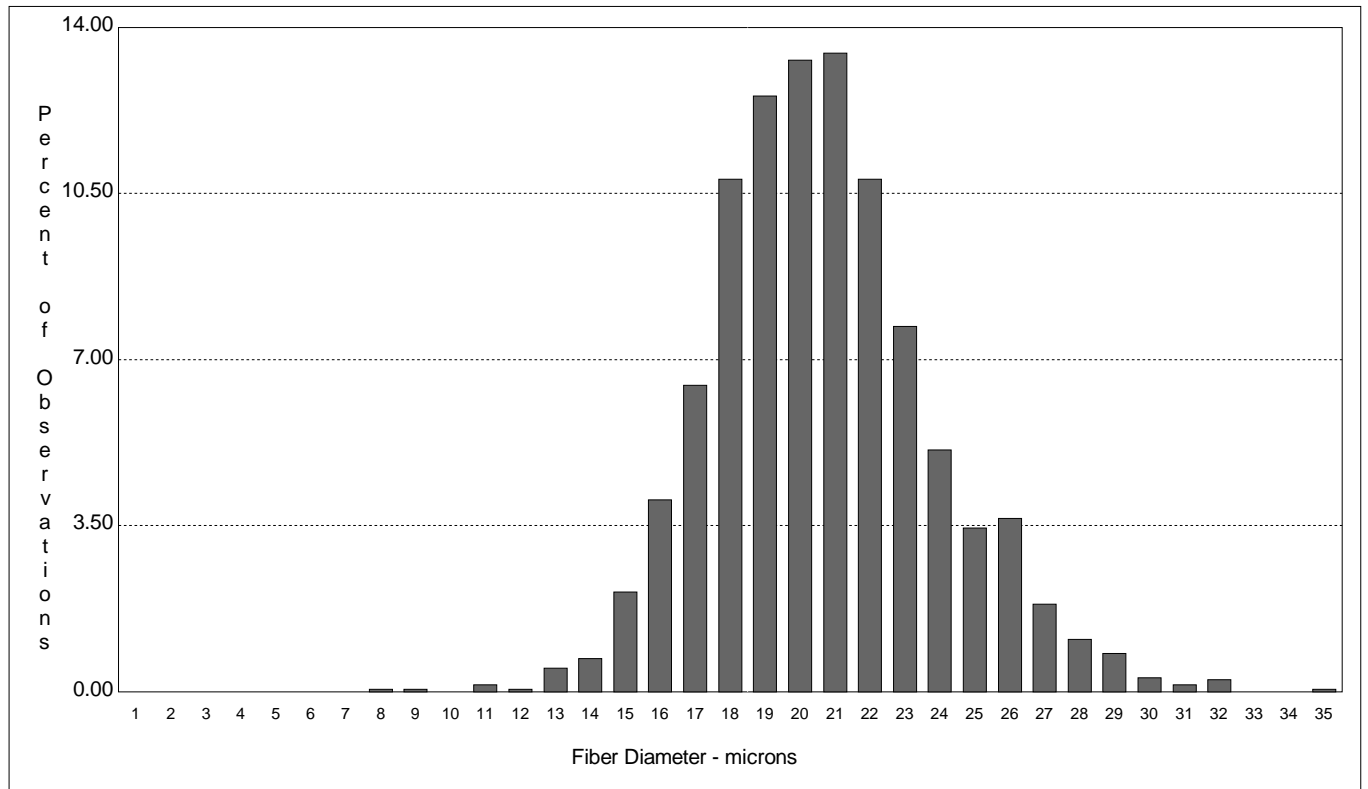

This Test Performed According to I.W.T.O Method 12